



## **PRODUCT INFORMATION & MANUAL**

**Human EMMPRIN/CD147 Valukine™ ELISA**

**VAL128**

For the quantitative determination of natural and recombinant human  
EMMPRIIN/CD147 concentrations

For research use only.  
Not for diagnostic or therapeutic procedures.

**Bio-Techne China Co. Ltd**

P: +86 (21) 52380373 P: 8009881270 F: +86 (21) 52381001  
**info.cn@bio-techne.com**

Please refer to the kit label for expiry date.  
Novus kits are guaranteed for 3 months from date of receipt

Version201910.1

## TABLE OF CONTENTS

<b>I. BACKGROUND</b> .....	2
<b>II. OVERVIEW</b> .....	3
<b>III. ADVANTAGES</b> .....	4
<b>IV. EXPERIMENT</b> .....	6
<b>V. KIT COMPONENTS AND STORAGE</b> .....	7
<b>VI. PREPARATION</b> .....	10
<b>VII. ASSAY PROCEDURE</b> .....	12
<b>VIII. REFERENCES</b> .....	14

## I. BACKGROUND

Extracellular matrix metalloproteinase (MMP) inducer (EMMPRIN), also known as basigin and CD147, is a 35-65 kDa, variably glycosylated, type I transmembrane protein that belongs to the immunoglobulin superfamily (1-4). Human EMMPRIN is 269 amino acids (aa) in length and contains a 24 aa signal sequence, a 183 aa extracellular domain (ECD), a 21 aa transmembrane (TM) segment and a 41 aa intracellular domain.

There are additional multiple potential isoform variants for EMMPRIN. Two that have been characterized are 205 and 176 aa in length. Notably, the 176 aa isoform heterodimerizes with the standard EMMPRIN isoform and down-modulates its activity. This is in contrast to EMMPRIN homodimers that show full biological activity (5). Human EMMPRIN (269 aa) shows 58%, 58%, 62% and 52% aa identity with mouse, rat, cow and chick EMMPRIN, respectively. It also shows 25% and 38% aa identity with the related proteins, embigin and neuroplastin (SDR-1), respectively.

EMMPRIN is expressed in areas of tissue remodeling, including endometrium, placenta, skin, and regions undergoing angiogenesis (1, 2, 6-9). It is also expressed on cells with high metabolic activity, such as lymphoblasts, macrophages and particularly tumor cells (2, 10). On such cells, EMMPRIN is often co-expressed with the amino acid transporter CD98h (11). EMMPRIN also interacts with caveolin-1 (via its C2-like domain), and this reduces the level of EMMPRIN glycosylation and subsequent EMMPRIN multimerization and activity (12). In addition, EMMPRIN is reported to complex with both annexin II and beta 1 integrins alpha 3 and alpha 6, an interaction that contributes to tumor growth and metastasis (13-15). Finally, the soluble calcium-binding protein S100A9 has now been identified as a ligand for EMMPRIN, and may mediate many of the tumorigenic activities attributed to EMMPRIN (16). EMMPRIN's TM sequence contains a charged aa (Glu), and a Pro important for intracellular interactions with cyclophilins (CyP) (3, 17, 18). CyPA (cyclosporin A receptor) and CyP60 interactions with the TM segment promote leukocyte inflammatory chemotaxis and surface expression of EMMPRIN, respectively (17, 18). An active 22kDa fragment can be shed from tumor cells by MT1-MMP (1). Tumor cells can also release active, full-length EMMPRIN in microvesicles (19, 20). Functionally, EMMPRIN is known to induce urokinase-type plasminogen activator (uPA), VEGF, hyaluronan and multiple MMPs (1, 2, 7-9).

## II. OVERVIEW

### A. PRINCIPLE OF THE ASSAY

This assay employs the quantitative sandwich enzyme immunoassay technique. An antibody specific for human EMMPRIN/CD147 has been pre-coated onto a microplate. Standards and samples are pipetted into the wells and any EMMPRIN/CD147 present is bound by the immobilized antibody. After washing away any unbound substances, a biotin-linked detect antibody specific for human EMMPRIN/CD147 are pipetted into the wells. After washing away any unbound substances, streptavidin-HRP is added. Following a wash to remove any unbound antibody-enzyme reagent, a substrate solution is added to the wells and color develops in proportion to the amount of EMMPRIN/CD147 bound in the initial step. The color development is stopped, and the intensity of the color is measured.

### B. LIMITATIONS OF THE PROCEDURE

- **FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.**
- This kit is suitable for cell culture supernate and serum.
- The kit should not be used beyond the expiration date on the kit label.
- Do not mix or substitute reagents with those from other lots or sources.
- If samples generate values higher than the highest standard, dilute the samples with Calibrator Diluent and repeat the assay.
- Any variation in operator, pipetting technique, washing technique, incubation time or temperature, and kit age can cause variation in binding.

### III. ADVANTAGES

#### A. PRECISION

**Intra-assay Precision** (Precision within an assay)

Three samples were tested twenty times on one plate to assess intra-assay precision.

**Inter-assay Precision** (Precision between assays)

Three samples were tested in twenty separate assays to assess inter-assay precision.

CELL CULTURE SUPERNATE / SERUM

Sample	Intra-assay Precision			Inter-assay Precision		
	1	2	3	1	2	3
Mean (pg/mL)	122.7	415.4	1746.0	124.4	438.4	1825.6
Standard Deviation	6.6	16.4	129.8	7.0	23.4	85.3
CV%	5.4	3.9	7.4	5.6	5.3	4.7

#### B. RECOVERY

The recovery of human EMMPRIN/CD147 spiked to three levels throughout the range of the assay in cell culture media was evaluated. The recovery ranged from 88.1-114.9% with an average of 107.3%.

#### C. SENSITIVITY

The minimum detectable dose (MDD) of EMMPRIN/CD147 is typically less than 6.84 pg/mL.

The MDD was determined by adding two standard deviations to the mean optical density value of twenty zero standard replicates and calculating the corresponding concentration.

#### D. CALIBRATION

This immunoassay is calibrated against a highly purified *NS0*-expressed recombinant human EMMPRIN/CD147 produced at R&D Systems®.

## E. LINEARITY

To assess the linearity of the assay, different samples containing or spiked with high concentrations of EMMPRIN/CD147 and diluted with Calibrator Diluent 1× to produce samples with values within the dynamic range of the assay.

Dilution	Average % of Expected	Range (%)
1:2	101.2	99.3-104.4
1:4	105.0	95.8-113.8
1:8	102.8	90.2-110.2
1:16	100.7	93.0-115.8

## F. SAMPLE VALUES

Five Serum samples were evaluated for the presence of EMMPRIN/CD147 in this assay. All samples measured ranged from 6510 to 10136 pg/mL with an average of 8760pg/mL.

## G. SPECIFICITY

The following factors prepared at 50 ng/mL were assayed and exhibited no cross-reactivity or interference.


Recombinant human :	Recombinant mouse :
CYPA	EMMPRIN
L1CAM/Fc Chimera	
MMP-1	
MMP-2	<b>Other factors :</b>
MMP-3	Hyaluronan(Medium MW)
MMP-9	
uPA	
VEGF	

## IV. EXPERIMENT

### EXAMPLE STANDARD

The standard curve is provided for demonstration only. A standard curve should be generated for each set of samples assayed.

#### CELL CULTURE SUPERNATE / SERUM

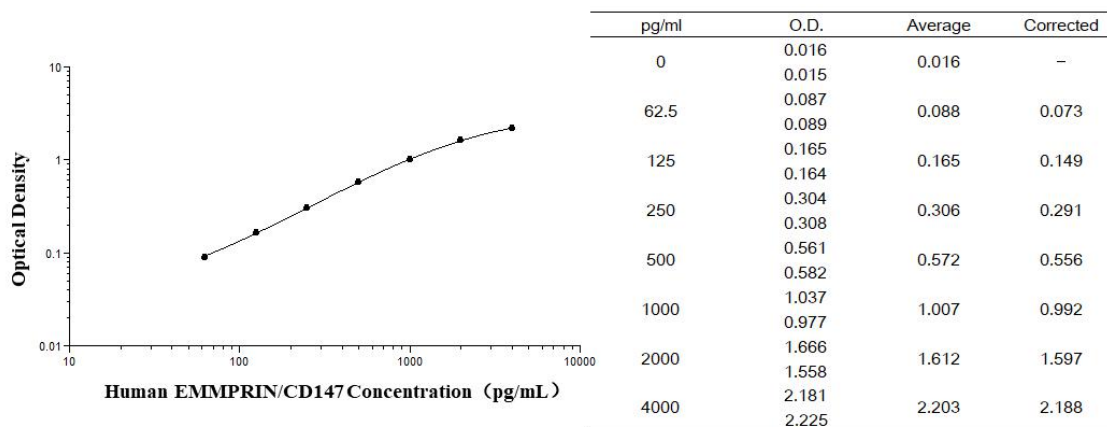

## V. KIT COMPONENTS AND STORAGE

### A. MATERIALS PROVIDED

Store the unopened kit at 2-8°C. Do not use past kit expiration date.

<b>Parts</b>	<b>Description</b>	<b>Size</b>
Human EMMPRIN/CD147 Microplate	96 well polystyrene microplate (12 strips of 8 wells) coated with a mouse antibody against human EMMPRIN/CD147.	1 plate
Human EMMPRIN/CD147 Standard	Recombinant human EMMPRIN/CD147 in a buffered protein base; lyophilized. Refer to the vial label for reconstitution volume.	2 vials
Human EMMPRIN/CD147 Detection Antibody	Biotinylated EMMPRIN/CD147 polyclonal antibody, lyophilized. Refer to the vial label for reconstitution volume.	1 vial
Streptavidin-HRP A (200×)	200× Streptavidin conjugated to horseradish peroxidase.	1 vial
Reagent Diluent (10×)	A 10× concentrated buffered protein base used to dilute detection antibody and HRP.	1 vial
Calibrator Diluent (2×)	A 2× concentrated buffered protein base used to dilute standard and samples.	1 vial
Detection Antibody Diluent (1×)	A buffered protein base used to dilute detection antibody.	1 vial
Wash Buffer Concentrate (25×)	A 25× concentrated solution of buffered surfactant with preservatives.	1 vial
Color Reagent A	Stabilized hydrogen peroxide.	1 vial
Color Reagent B	Stabilized chromogen (tetramethylbenzidine).	1 vial
Stop Solution	2N sulfuric acid.	1 vial
Plate Sealers	Adhesive strips.	3 strips



## B. STORAGE

<b>Unopened Kit</b>	Store at 2-8 °C. Do not use past kit expiration date.	
<b>Opened/ Reconstituted Reagents</b>	Streptavidin-HRP A	May be stored for up to 1 month at 2-8 °C.*
	Diluted Wash Solution	
	Unmixed Color Reagent A	
	Unmixed Color Reagent B	
	Stop Solution	
	Standard	Prepare fresh for each assay.
	Detection Antibody	Aliquot and store for up to 1 month at -20 °C in a manual defrost freezer. *
	Reagent Diluent (10×)	May be stored for up to 1 month at 2-8 °C.*
		Use and discard diluted Reagent Diluent (1×). Prepare fresh for each assay.
	Calibrator Diluent (2×)	May be stored for up to 1 month at 2-8 °C.*
Use and discard diluted Reagent Diluent (1×). Prepare fresh for each assay.		
Detection Antibody Diluent (1×)	May be stored for up to 1 month at 2-8 °C.*	
Microplate Wells	Return unused wells to the foil pouch containing the desiccant pack, reseal along entire edge of zip-seal. May be stored for up to 1 month at 2-8 °C.*	

\* Provided this is within the expiration date of the kit.

### **C. OTHER SUPPLIES REQUIRED**

- ◆ Microplate reader capable of measuring absorbance at 450 nm, with the correction wavelength set at 540 nm or 570 nm.
- ◆ Pipettes and pipette tips.
- ◆ Deionized or distilled water.
- ◆ Squirt bottle, manifold dispenser, or automated microplate washer.
- ◆ Test tubes for dilution of standards.
- ◆ 100mL and 500 mL graduated cylinder.

### **D. PRECAUTION**

- ◆ Some components in this kit contain a preservative which may cause an allergic skin reaction. Avoid breathing mist.
- ◆ Color Reagent B may cause skin, eye, and respiratory irritation. Avoid breathing fumes.
- ◆ The Stop Solution provided with this kit is an acid solution.
- ◆ Wear protective gloves, clothing, eye, and face protection. Wash hands thoroughly after handling.

## VI. PREPARATION

### A. SAMPLE COLLECTION AND STORAGE

**Cell Culture Supernates** - Remove particulates by centrifugation and assay immediately or aliquot and store samples at  $\leq -20^{\circ}\text{C}$ . Avoid repeated freeze-thaw cycles.

**Serum** - Use a serum separator tube (SST) and allow samples to clot for 30 minutes at room temperature before centrifugation for 15 minutes at 1000 x g. Remove serum and assay immediately or aliquot and store samples at  $\leq -20^{\circ}\text{C}$ . Avoid repeated freeze-thaw cycles.

### B. SAMPLE PREPARATION

Serum samples require a 20-fold dilution prior to the assay. A suggested 20-fold dilution is 10  $\mu\text{L}$  of sample + 190  $\mu\text{L}$  of Calibrator Diluent (1 $\times$ ).

### C. REAGENT PREPARATION

**Bring all reagents to room temperature before use.**

***Note:** High concentrations of EMMPRIN//CD147 are found in saliva. It is recommended that a face mask and gloves be used to protect kit reagents from contamination.*

**Wash Buffer** - If crystals have formed in the concentrate, warm to room temperature and mix gently until the crystals have completely dissolved. Dilute 20 mL of Wash Buffer Concentrate (25 $\times$ ) into deionized or distilled water to prepare 500 mL of Wash Buffer.

**Reagent Diluent (1 $\times$ )** - Add 3 mL of Reagent Diluent (10 $\times$ ) into 27 mL of deionized or distilled water to prepare 30 mL of Reagent Diluent (1 $\times$ ).

**Detection Antibody- Reconstitution Volume refer to vial label with Reagent Diluent (1 $\times$ ).** Aliquot and store if needed. Dilute stock solution in Detection Antibody Diluent (1 $\times$ ) to the working concentration of 50 ng/mL. Prepare at least 15 minutes prior to use.

**Streptavidin-HRP A (1 $\times$ )** - Dilute to the working concentration specified on the vial label using Reagent Diluent (1 $\times$ ).


**Substrate Solution** - Color Reagent A and B should be mixed together in equal volumes within 15 minutes of use. Protect from light. 100  $\mu\text{L}$  of the resultant mixture is required per well.

**EMMPRIIN/CD147 Standard – Refer to the vial label for the reconstitution volume\* using Calibrator Diluent 1 $\times$ .** This reconstitution produces a stock solution of 8000

pg/mL. Allow the standard to sit for a minimum of 15 minutes with gentle agitation prior to making dilutions.

\*if you have any question, please seek help from our Technical Support.

**Pipette 300  $\mu$ L of Calibrator Diluent 1 $\times$  into each tube.** Use the stock solution to produce a dilution series (below). Mix each tube thoroughly before the next transfer. The 4000 pg/mL standard serves as the high standard. The **Calibrator Diluent 1 $\times$**  serves as the zero standard (0 pg/mL).

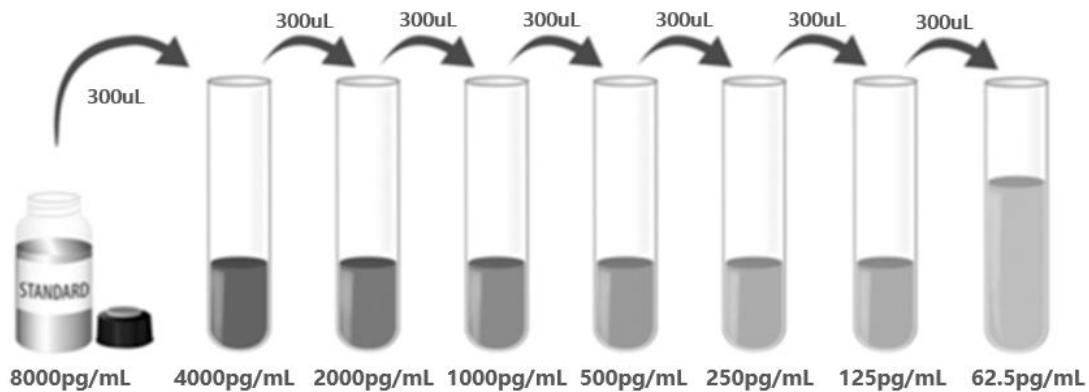

#### D. TECHNICAL HINTS

- When mixing or reconstituting protein solutions, always avoid foaming.
- To avoid cross-contamination, change pipette tips between additions of each standard level, between sample additions, and between reagent additions. Also, use separate reservoirs for each reagent.
- It is recommended that the samples be pipetted within 15 minutes.
- To ensure accurate results, proper adhesion of plate sealers during incubation steps is necessary.
- Substrate Solution should remain colorless until added to the plate. Keep Substrate Solution protected from light. Substrate Solution should change from colorless to gradations of blue.
- Stop Solution should be added to the plate in the same order as the Substrate Solution. The color developed in the wells will turn from blue to yellow upon addition of the Stop Solution. Wells that are green in color indicate that the Stop Solution has not mixed thoroughly with the Substrate Solution.

## VII. ASSAY PROCEDURE

**Bring all reagents and samples to room temperature before use. It is recommended that all samples and standards be assayed in duplicate.**

*Note: High concentrations of EMMPRIN/CD147 are found in saliva. It is recommended that a face mask and gloves be used to protect kit reagents from contamination.*

1. Prepare all reagents and working standards as directed in the previous sections.
2. Remove excess microplate strips from the plate frame, return them to the foil pouch containing the desiccant pack, and reseal.
3. Add 100  $\mu$ L of Standard, or prepared sample per well. Cover with the adhesive strip provided. Incubate for 2 hours at room temperature. A plate layout is provided for a record of standards and samples assayed. (Samples may require dilution. See Sample Preparation section.)
4. Aspirate each well and wash, repeating the process three times for a total of four washes. Wash by filling each well with Wash Solution (400  $\mu$ L) using a squirt bottle, manifold dispenser, or autowasher. Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels.
5. Add 100  $\mu$ L of the Detection Antibody diluted in Detection Antibody Diluent, to each well. Cover with a new adhesive strip and incubate 2 hours at room temperature.
6. Repeat the aspiration/wash as in step 4.
7. Add 100  $\mu$ L of the working dilution of Streptavidin-HRP A to each well. Cover the plate and incubate for 20 minutes at room temperature. Avoid placing the plate in direct light.
8. Repeat the aspiration/wash as in step 4.
9. Add 100  $\mu$ L of Substrate Solution to each well. Incubate for 30 minutes at room temperature. Avoid placing the plate in direct light.
10. Add 50  $\mu$ L of Stop Solution to each well. Gently tap the plate to ensure thorough mixing.
11. Determine the optical density of each well immediately, using a microplate reader set to 450 nm. If wavelength correction is available, set to 540 nm or 570 nm. If wavelength correction is not available, subtract readings at 540 nm or 570 nm from the readings at 450 nm. This subtraction will correct for optical imperfections in the plate. Readings made directly at 450 nm without correction may be higher and less accurate.

## 12. CALCULATION OF RESULTS

Average the duplicate readings for each standard, control, and sample and subtract the average zero standard optical density (O.D.).

Create a standard curve by reducing the data using computer software capable of generating a four parameter logistic (4-PL) curve-fit. As an alternative, construct a standard curve by plotting the mean absorbance for each standard on the y-axis against the concentration on the x-axis and draw a best fit curve through the points on the graph. The data may be linearized by plotting the log of the EMMPRIN/CD147 concentrations versus the log of the O.D. and the best fit line can be determined by regression analysis. This procedure will produce an adequate but less precise fit of the data.

If samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.

## VIII. REFERENCES

1. Gabison, E. E. et al. (2005) *Biochimie* 87:361.
2. Yurchenko, V. et al. (2006) *Immunology* 117:301.
3. Kasinrerker, W. et al. (1992) *J. Immunol.* 149:847.
4. Iacono, K.T. et al. (2007) *Exp. Mol. Pathol.* 83:283.
5. Liao, C-G. et al. (2011) *Mol. Cell. Biol.* 31:2591.
6. Riethdorf, S. et al. (2006) *Int. J. Cancer* 119:1800.
7. Braundmeier, A. G. et al. (2006) *J. Clin. Endocrinol. Metab.* 91:2358.
8. Tang, Y. et al. (2006) *Mol. Cancer Res.* 4:371.
9. Quemener, C. et al. (2007) *Cancer Res.* 67:9.
10. Wilson, M. C. et al. (2005) *J. Biol. Chem.* 280:27213.
11. Xu, D. and M. E. Hemler, (2005) *Mol. Cell. Proteomics* 4:1061.
12. Tang, W. et al. (2004) *Mol. Biol. Cell* 15:4043.
13. Zhao, P. et al. (2010) *Cancer Sci.* 101:387.
14. Dai, J. et al. (2009) *BMC Cancer* 9:337.
15. Li, Y. et al. (2012) *J. Biol. Chem.* 287:4759.
16. Hibino, T. et al. (2013) *Cancer Res.* 73:172.
17. Arora, K. et al. (2005) *J. Immunol.* 175:517.
18. Pushkarsky, T. et al. (2005) *J. Biol. Chem.* 280:27866.
19. Egawa, N. et al. (2006) *J. Biol. Chem.* 281:37576.
20. Sidhu, S. S. et al. (2004) *Oncogene* 23:956.

**PLATE LAYOUT**

Use this plate layout to record standards and samples assayed.

<b>1</b>																	
<b>2</b>																	
<b>3</b>																	
<b>4</b>																	
<b>5</b>																	
<b>6</b>																	
<b>7</b>																	
<b>8</b>																	
<b>9</b>																	
<b>10</b>																	
<b>11</b>																	
<b>12</b>																	
	<b>A</b>	<b>B</b>	<b>C</b>	<b>D</b>	<b>E</b>	<b>F</b>	<b>G</b>	<b>H</b>									





## 产品信息及操作手册

人 EMMPRIN/CD147 Valukine™ ELISA 试剂盒

目录号: VAL128

适用于定量检测天然和重组人 EMMPRIN/CD147 的浓度

科研专用，不可用于临床诊断

**Bio-Techne China Co. Ltd**

P: +86 (21) 52380373 P: 8009881270 F: +86 (21) 52381001

**info.cn@bio-techne.com**

有效期详见试剂盒包装标签

Novus 试剂盒确保在你收货日期 3 个月内有效

## 目录

I. 背景	18
II. 概述	19
III. 优势	20
IV. 实验	22
V. 试剂盒组成及储存	23
VI. 实验前准备	25
VII. 操作步骤	27
VIII. 参考文献	28

## I. 背景

细胞外基质金属蛋白酶(MMP)诱导剂(EMMPRIN), 也被称为 **basigin** 和 **CD147**, 是一种不同糖基化的, 35-65 kDa 的 I 型跨膜蛋白, 属于免疫球蛋白超家族(1-4)。人 EMMPRIN 全长为 269 个氨基酸 (aa), 包含 24 aa 的信号序列、183 个 aa 的胞外结构域(ECD)、21 个 aa 的跨膜段和 41 个 aa 的胞内段。EMMPRIN 还有多个潜在的亚型变体。其中两个已被鉴定的长度是 205 和 176 aa 的变体。值得注意的是, 176 aa 异构体与标准 EMMPRIN 形成异二聚体并能使其活性下调。这与 EMMPRIN 同型二聚体形成鲜明对比, 后者具有完全的生物活性(5)。人 EMMPRIN (269 aa) 与小鼠、大鼠、牛、鸡 EMMPRIN 的一致性分别为 58%、58%、62%和 52%。与相关蛋白 **embigin** 和 **neuroplastin (SDR-1)** 的 aa 一致性分别为 25%和 38%。

EMMPRIN 在组织重塑区域表达, 包括子宫内膜、胎盘、皮肤和进行血管生成的区域(1,2,6-9)。也在具有高代谢活性的细胞中表达, 如成淋巴细胞、巨噬细胞, 尤其是肿瘤细胞(2,10)。在这些细胞中, EMMPRIN 常与氨基酸转运体 **CD98h** 共表达(11)。EMMPRIN 还与 **caveolin-1** 相互作用(通过其 C2 样结构域), 这降低了 EMMPRIN 糖基化水平及后续 EMMPRIN 多聚化和活性 (12)。此外, EMMPRIN 被报道能与 **annexin II**、 $\beta$ -1 整合素的  $\alpha$ -3 和  $\alpha$ -6 结合, 这种相互作用有助于肿瘤生长和转移(13-14)。最后, 可溶性钙结合蛋白 **S100A9** 现已被鉴定为 EMMPRIN 的配体, 并可能介导许多 EMMPRIN 的致瘤活性(16)。EMMPRIN 的 TM 序列包含一个带电荷的 aa (Glu), 以及一个对细胞内与环蛋白(CyP)相互作用很重要的 Pro(3,17,18)。CyPA(环孢素 A 受体)和 CyP60 的 TM 段的相互作用分别促进白细胞炎症趋化和 EMMPRIN 的表面表达(17,18)。MT1 - MMP 可以从肿瘤细胞中分离出具有活性的 22kDa 片段(1)。肿瘤细胞也可以在微泡中释放具有活性的全长 EMMPRIN(19,20)。在功能上, EMMPRIN 可诱导尿激酶型纤溶酶原激活剂(uPA)、VEGF、透明质酸和多种 MMPs(1,2,7-9)。

## II. 概述

### A. 检测原理

本实验采用双抗体夹心 ELISA 法。抗人 EMMPRIN/CD147 捕获抗体包被于微孔板上，经过孵育，样品和标准品中的 EMMPRIN/CD147 会与固定在板上的抗体结合，游离的成分被洗去；接着加入生物素化的抗人 EMMPRIN/CD147 检测抗体进行孵育，洗涤去除未结合的物质后，加入链霉亲和素标记的辣根过氧化物酶(streptavidin-HRP) 孵育。洗涤后，加入显色底物，避光显色。溶液颜色与结合的目标蛋白成正比；加入终止液；用酶标仪测定吸光度。

### B. 检测局限

- ◆ 仅供科研使用，不可用于体外诊断；
- ◆ 该试剂盒适用于细胞培养上清样本和血清样本；
- ◆ 请在试剂盒有效期内使用；
- ◆ 不同试剂盒及不同批号试剂盒的组分不能混用；
- ◆ 样本值若大于标准曲线的最高值，应将样本用标准品稀释剂（1×）稀释后重新检测；
- ◆ 检测结果的不同可由多种因素引起，包括实验人员的操作、移液器的使用方式、洗板技术、反应时间或温度、试剂盒的储存等。

### III. 优势

#### A. 精确度

**板内精确度**（同一板内不同孔间的精确度）

已知浓度的三个样本，在同一板内分别检测 20 次，以确定板内精确度。

**板间精确度**（不同板之间的精确度）

已知浓度的三个样本，在不同板中分别检测 20 次，以确定板间精确度。

细胞培养上清/血清

样本	板内精确度			板间精确度		
	1	2	3	1	2	3
平均值 (pg/mL)	122.7	415.4	1746.0	124.4	438.4	1825.6
标准差	6.6	16.4	129.8	7.0	23.4	85.3
CV%	5.4	3.9	7.4	5.6	5.3	4.7

#### B. 回收率

在细胞培养基样本中掺入检测范围内不同水平的人 EMMPRIN/CD147，测定其回收率。回收率范围在 88.1-114.9%，平均回收率在 107.3%。

#### C. 灵敏度

人 EMMPRIN/CD147 的最低可测剂量（MDD）一般小于 6.84 pg/mL。

MDD 是根据 20 个重复的零标准品孔的吸光度值的平均值加两倍标准差计算得到的相对对应浓度。

#### D. 校正

此 ELISA 试剂盒经由 R&D Systems® 生产的 NS0 表达的高纯度重组人 EMMPRIN/CD147 蛋白所校正。

#### E. 线性

不同的样本中含有或掺入高浓度的人 EMMPRIN/CD147，然后用标准品稀释剂（1×）将样本稀释到检测范围内，测定其线性。

稀释倍数	平均期待值 (%)	范围 (%)
1:2	101.2	99.3-104.4
1:4	105.0	95.8-113.8
1:8	102.8	90.2-110.2
1:16	100.7	93.0-115.8

## F. 样本值

使用本试剂盒检测了 5 份人血清样本中 EMMPRIN/CD147 的水平。5 份样本的检测值在 6510 -10136 pg/mL 之间，平均值为 8760 pg/mL。

## G. 特异性

对制备的 50 ng/mL 的下列因素进行了测定，无交叉反应或干扰。

### 重组人蛋白：

CYPA

L1CAM/Fc Chimera

MMP-1

MMP-2

MMP-3

MMP-9

uPA

VEGF

### 重组小鼠蛋白：

EMMPRIN

### 其它重组蛋白：


Hyaluronan(Medium MW)

## IV. 实验

### 标准曲线实例

该标准曲线数据仅供参考，每次实验应绘制其对应的标准曲线。

细胞培养上清/血清

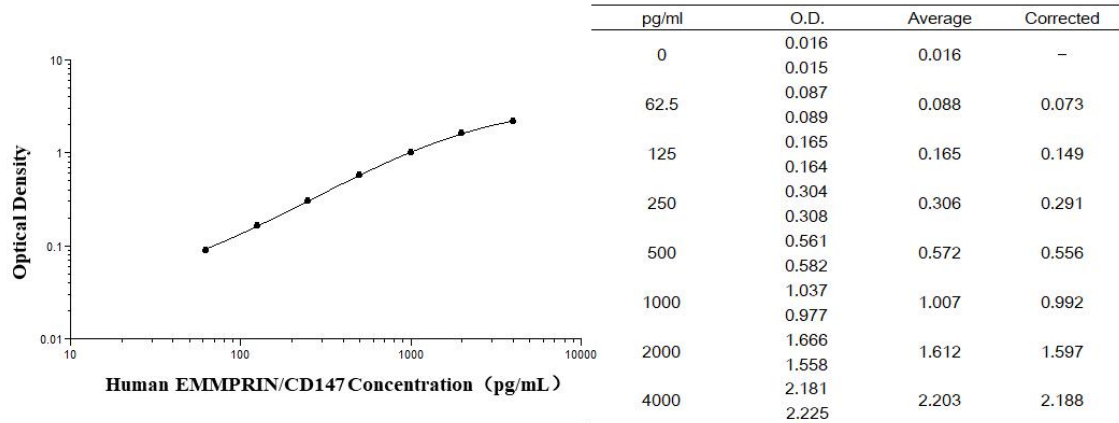

## V. 试剂盒组成及储存

### A. 试剂盒组成

组成	描述	规格
Human EMMPRIN/CD147 Microplate	包被小鼠抗人 EMMPRIN/CD147 抗体的 96 孔聚苯乙烯板, 8 孔×12 条	1 块板
Human EMMPRIN/CD147 Standard	标准品 (冻干粉), 参考瓶标签进行重溶	2 瓶
Human EMMPRIN/CD147 Detection Antibody	生物素化的 EMMPRIN/CD147 检测抗体, 冻干粉, 参考瓶标签进行重溶	1 瓶
Streptavidin-HRP A (200×)	200×浓缩的链霉亲和素标记的 HRP	1 瓶
Reagent Diluent (10×)	浓缩的试剂稀释液 (10 ×)	1 瓶
Calibrator Diluent (2×)	标准品稀释剂 (2 ×)	1 瓶
Detection Antibody Diluent (1×)	检测抗体稀释液 (1 ×)	1 瓶
Wash Buffer Concentrate (25×)	浓缩洗涤缓冲液 (25 ×)	1 瓶
Color Reagent A	显色液 A	1 瓶
Color Reagent B	显色液 B	1 瓶
Stop Solution	终止液	1 瓶
Plate Sealers	封板膜	3 张

### B. 试剂盒储存

未开封试剂盒	2-8℃储存; 请在试剂盒有效期内使用	
已打开, 稀释或重溶的试剂	链霉亲和素-HRP A	2-8℃储存, 最多 30 天*
	洗涤缓冲液 (1×)	
	显色剂 A	
	显色剂 B	
	终止液	
	标准品	使用时新鲜配制*
	检测抗体	分装, -20℃储存, 最多 30 天*
	试剂稀释液 (10×)	2-8℃储存, 最多 30 天* 请每次使用新鲜配制的 1×稀释液
	标准品稀释剂 (2×)	2-8℃储存, 最多 30 天* 请每次使用新鲜配制的 1×稀释液
	检测抗体稀释液 (1×)	2-8℃储存, 最多 30 天*
包被的微孔板条	将未用的板条放回带有干燥剂的铝箔袋内, 密封: 2-8℃储存, 最多 30 天*	

\*必须在试剂盒有效期内



### C. 实验所需自备试验器材

- ◆ 酶标仪（可测量 450 nm 检测波长的吸收值及 540 nm 或 570 nm 校正波长的吸收值）
- ◆ 高精度加液器及一次性吸头
- ◆ 蒸馏水或去离子水
- ◆ 洗瓶（喷瓶）、多通道洗板器或自动洗板机
- ◆ 用来稀释标准品的试管
- ◆ 100 mL 及 500 mL 量筒

### D. 注意事项

- ◆ 试剂盒中的终止液是酸性溶液，使用时请做好眼镜、手、面部及衣服的保护。
- ◆ 试剂盒中的一些组分，可能引起皮肤、眼睛和呼吸道刺激或皮肤过敏反应。避免吸入。
- ◆ 实验穿戴防护衣服、手套、眼睛和脸的保护罩。使用后请彻底洗手。

## VI. 实验前准备

### A. 样品收集及储存

**细胞培养上清液：**颗粒物应离心去除；立刻检测样本。样本收集后若不及时检测，需按一次使用量分装，冻存于-20℃冰箱内，避免反复冻融。

**血清样本：**用血清分离管(SST)分离血清。使血样室温凝集30分钟，然后1000 x g离心15分钟。吸取血清样本之后即刻用于检测，或者分装，-20℃贮存备用。避免反复冻融。

### B. 样本准备工作

血清样本需要用标准品稀释剂（1×）20倍稀释后进行检测，例如：10μL血清+190μL标准品稀释剂（1×）。

### C. 检测前准备工作

使用前请将所有试剂放置于室温。

**注：**唾液中含有高浓度的EMMPRIN/CD147，为避免污染，实验时请戴口罩、手套。

**洗涤液：**从冰箱中取出的浓缩洗涤液可能有结晶，属于正常现象；放置室温，轻摇混匀，待结晶完全溶解后再配制洗涤液。可将20 mL浓缩洗涤液用蒸馏水或去离子水稀释配置成500 mL工作浓度的洗涤液。可4℃存储。

**试剂稀释液（1×）：**加3 mL试剂稀释液（10×）至27 mL蒸馏水或去离子水中，制成30 mL试剂稀释液（1×）。

**检测抗体：**参考检测抗体瓶标签指示，用试剂稀释液（1×）将冻干粉进行重溶。再用检测抗体稀释液（1×）稀释至工作浓度50 ng/mL，至少在使用前15分钟准备。

**标准品稀释剂（1×）：**使用蒸馏水或去离子水稀释配置成标准品稀释剂（1×）。


**链霉亲和素-HRP A：**用试剂稀释液（1×）将链霉亲和素-HRP A（200×）稀释至工作浓度链霉亲和素-HRP A（1×）。

**显色剂：**按试验所需用量（100 μL/孔）将显色液A和显色液B等体积混合，避光保存，现用现配，须在15分钟内使用。

**标准品：**参照冻干标准品瓶身注明的方式重溶冻干标准品\*，得到浓度为8000 pg/mL标准品母液。轻微震荡至少15分钟，使其充分溶解。

**\*如有疑问，请咨询我们的技术支持。**

每个稀释管中加入300 μL标准品稀释剂（1×）。将标准品母液参照下图做系列稀释，每管须充分混匀后再移液到下一管。4000 pg/mL管作标准曲线最高点，标准品稀释剂（1×）可用作标准品零点（0 pg/mL）。

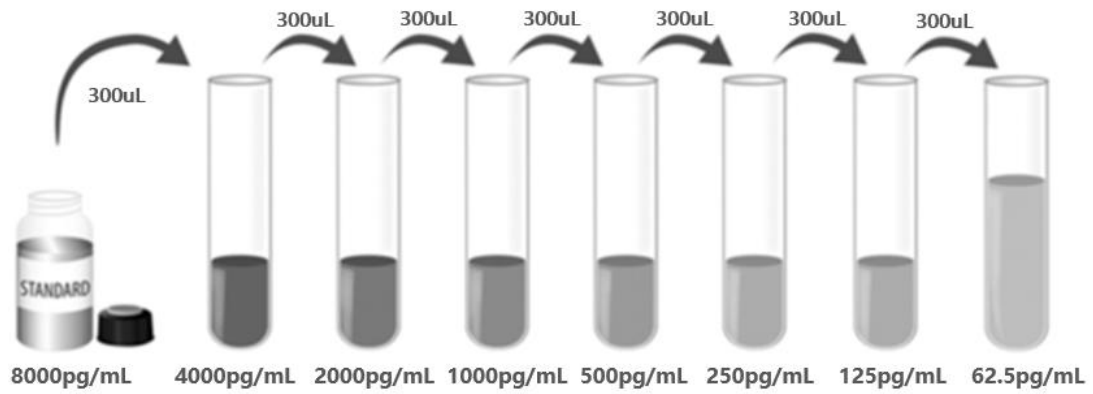

#### D. 技术小提示

- ◆ 当混合或重溶蛋白液时，尽量避免起沫；
- ◆ 为了避免交叉污染，配置不同浓度标准品、上样、加不同试剂都需要更换枪头。另外不同试剂请分别使用不同的移液槽；
- ◆ 建议 15 分钟内完成一块板的上样；
- ◆ 每次孵育时，正确使用封板膜可保证结果的准确性；
- ◆ 混合后的显色剂在上板前应为无色，请避光保存；加入微孔板后，将由无色变成不同深度的蓝色；
- ◆ 终止液上板顺序应同显色底物上板顺序一致；加入终止液后，孔内颜色由蓝变黄；若孔内有绿色，则表明孔内液体未混匀，请充分混合。

## VII. 操作步骤

使用前请将所有试剂和样本放置于室温，建议所有的实验样本和标准品做复孔检测。

**注：唾液中**含有高浓度的 **EMMPRIN/CD147**，为避免污染，实验时请戴口罩、手套。

1. 按照上一节的说明，准备好所有需要的试剂和标准品；
2. 从已平衡至室温的密封袋中取出微孔板，未用的板条请放回铝箔袋内，重新封口；
3. 分别将不同浓度标准品，实验样本或者质控品加入相应孔中，每孔 100  $\mu\text{L}$ 。用封板膜封住反应孔，室温孵育 2 小时。说明书提供了一张 96 孔模板图，可用于记录标准品和试验样本的板内位置；（样本需要稀释，详情参见样本制备部分。）
4. 将板内液体吸去，使用洗瓶、多通道洗板器或自动洗板机洗板。每孔加洗涤液 400  $\mu\text{L}$ ，然后将板内洗涤液吸去。重复操作 3 次，共洗 4 次。每次洗板尽量吸去残留液体会有助于得到好的实验结果。最后一次洗板结束，请将板内所有液体吸干或将板倒置，在吸水纸拍干所有残留液体；
5. 在每个微孔内加入 100  $\mu\text{L}$  配置好的检测抗体。用封板膜封住反应孔，室温孵育 2 小时；
6. 重复第 4 步洗板操作；
7. 在每个微孔内加入 100  $\mu\text{L}$  稀释好的链霉亲和素- HRP A 工作液。用封板膜封住反应孔，室温孵育 20 分钟，**注意避光**；
8. 重复第 4 步洗板操作；
9. 在每个微孔内加入 100  $\mu\text{L}$  显色剂，室温孵育 30 分钟，**注意避光**；
10. 在每个微孔内加入 50  $\mu\text{L}$  终止液，请轻拍微孔板，使溶液混合均匀。孔内溶液颜色会从蓝色变为黄色；
11. 加入终止液后 30 分钟内，使用酶标仪测量 450 nm 的吸光度值，设定 540 nm 或 570 nm 作为校正波长。如果没有使用双波长校正，结果准确度可能会受影响；
12. **计算结果：**将每个标准品和样品的校正吸光度值（ $\text{OD}_{450}-\text{OD}_{540}/\text{OD}_{570}$ ），复孔读数取平均值，然后减去平均零标准品 OD 值。使用计算机软件作四参数逻辑（4-PL）曲线拟合创建标准曲线。另一种方法是，可以通过绘制标准品浓度做对数与相应 OD 值对数生成曲线，并通过回归分析确定最佳拟合线。通过样本的 OD 值，可从标准曲线上得到样本中人 EMMPRIN/CD147 的浓度。如果样品被稀释，从标准曲线读取的浓度必须乘以稀释倍数。

## VIII. 参考文献

1. Gabison, E. E. et al. (2005) *Biochimie* 87:361.
2. Yurchenko, V. et al. (2006) *Immunology* 117:301.
3. Kasinrerker, W. et al. (1992) *J. Immunol.* 149:847.
4. Iacono, K.T. et al. (2007) *Exp. Mol. Pathol.* 83:283.
5. Liao, C-G. et al. (2011) *Mol. Cell. Biol.* 31:2591.
6. Riethdorf, S. et al. (2006) *Int. J. Cancer* 119:1800.
7. Braundmeier, A. G. et al. (2006) *J. Clin. Endocrinol. Metab.* 91:2358.
8. Tang, Y. et al. (2006) *Mol. Cancer Res.* 4:371.
9. Quemener, C. et al. (2007) *Cancer Res.* 67:9.
10. Wilson, M. C. et al. (2005) *J. Biol. Chem.* 280:27213.
11. Xu, D. and M. E. Hemler, (2005) *Mol. Cell. Proteomics* 4:1061.
12. Tang, W. et al. (2004) *Mol. Biol. Cell* 15:4043.
13. Zhao, P. et al. (2010) *Cancer Sci.* 101:387.
14. Dai, J. et al. (2009) *BMC Cancer* 9:337.
15. Li, Y. et al. (2012) *J. Biol. Chem.* 287:4759.
16. Hibino, T. et al. (2013) *Cancer Res.* 73:172.
17. Arora, K. et al. (2005) *J. Immunol.* 175:517.
18. Pushkarsky, T. et al. (2005) *J. Biol. Chem.* 280:27866.
19. Egawa, N. et al. (2006) *J. Biol. Chem.* 281:37576.
20. Sidhu, S. S. et al. (2004) *Oncogene* 23:956.