

INTENDED USE

The MagCelect Mouse CD3⁺ T Cell Isolation Kit is designed to isolate CD3⁺ T cells via a negative selection principle. The resulting cell preparation is highly enriched with CD3⁺ T cells. Typical purity of recovered CD3⁺ T cells ranges from 90-98%.

BACKGROUND

R&D Systems® MagCelect products are designed for the isolation of cells in a "liquid phase". R&D Systems MagCelect technology is based on the use of ferrofluids or magnetic nanoparticles that have no magnetic memory (superparamagnetic), and behave like colloidal particles. This feature allows the ferrofluids to remain in solution without the need for mixing and additionally allows for efficient diffusion kinetics during the binding reaction. The proprietary manufacturing technology of MagCelect Ferrofluids generates particles with higher ligand binding capacity per mass compared to many other larger diameter magnetic particles.

PRINCIPLE OF SELECTION

A mononuclear cell suspension is first incubated with the MagCelect Mouse CD3⁺ T Cell Biotinylated Antibody Cocktail which targets the unwanted cells. MagCelect Streptavidin Ferrofluid is next added to the reaction and the streptavidin coated nanoparticles interact with biotinylated antibody tagged cells. The tube containing the cell suspension is then placed within a magnetic field. Magnetically tagged cells will migrate toward the magnet (unwanted cell fraction), leaving the untagged cells or desired cell population in suspension to be harvested by aspiration while the tube remains in the magnetic field. The enriched cell preparation is then available for a variety of applications including tissue culture, immune status monitoring and flow cytometry.

MATERIALS PROVIDED & STORAGE CONDITIONS

Store the unopened kit at 2-8 °C. **DO NOT FREEZE.**

This kit contains sufficient reagents to process 1 x 10⁹ total cells.

PART	PART #	DESCRIPTION	STORAGE OF OPENED/DILUTED MATERIAL
Mouse CD3 ⁺ T Cell Biotinylated Antibody Cocktail	860041	1 mL of a phosphate buffered solution containing BSA and preservative.	May be stored at 2-8 °C when handled aseptically.*
Streptavidin Ferrofluid	860127	1.25 mL of a solution containing BSA and preservatives.	
10X Buffer	860040	10 mL of a 10-fold concentrated buffer.	May be stored for up to 24 hours at 2-8 °C after dilution.*

* Provided this is within the expiration date of the kit.

OTHER SUPPLIES REQUIRED

- MagCelect Magnet (R&D Systems, Catalog # MAG997)
- 12 x 75 mm (5 mL) or 17 x 100 mm (15 mL) polystyrene round bottom tubes
- Sterile Pasteur pipettes or transfer pipettes (ThermoFisher, Catalog # 13-711-9B or equivalent)
- Sterile distilled or deionized water

PRECAUTION

Some components of this kit contain sodium azide, which may react with lead and copper plumbing to form explosive metallic azides. Flush with large volumes of water during disposal.

CELL PREPARATION

1. Gently tease apart the mouse spleen(s) in order to generate a single cell suspension in Hanks' Balanced Salt Solution (HBSS) (or other preferred media) supplemented with 10% bovine serum. To remove cell clumps and/or debris pass the suspended cells through a 40-70 μm nylon cell strainer.
2. Wash the cells once by filling a 15 or 50 mL centrifuge tube with HBSS + 10% serum and spinning the cells for 10 minutes at 200 x g (use a 50 mL tube when processing more than 2 spleens).
3. Decant the supernatant, disrupt the cell pellet by "racking" the tube, resuspend the cells in R&D Systems® Mouse Erythrocyte Lysing Kit (Catalog # WL2000) that has been diluted to 1X strength with sterile distilled or deionized water and quickly vortex the tube (*using 2 mL of 1X M-Lyse Buffer per processed spleen is recommended*).
4. Incubate the cells for 10 minutes at room temperature and then fill the tube with 1X Wash Buffer from the Lysing kit.
Note: *The wash buffer must also be diluted with sterile water to 1X strength prior to use.*
5. Spin the cells for 10 minutes at 200 x g and then resuspend the cells in a small volume of cold 1X MagCelect™ Buffer (prepared as described in step 1 of the Cell Selection Procedure).
6. Perform a cell count and then adjust the cell concentration to 2×10^8 cells per mL with cold 1X MagCelect Buffer.
7. Continue the cell selection by referring to step # 1 of the cell selection procedure.

CELL SELECTION PROCEDURE


This procedure is for processing of 2×10^8 total cells using 5 mL tubes and the MagCelect Magnet. For processing other cell numbers please refer to the Technical Hints section on this insert. Cells and reagents should be kept cold using an ice bath or a refrigerator. **Reaction incubations must be carried out at 2-8 °C in a refrigerator and not in an ice bath in order to avoid excessively low temperatures that can slow the kinetics of the optimized reactions.**

1. Prepare 10 mL of 1X MagCelect Buffer for each 2×10^8 cells to be processed by mixing 1 mL of 10X Buffer with 9 mL sterile deionized or distilled water. The 1X MagCelect Buffer should be kept on ice or refrigerated and used within 24 hours.
2. Prepare a single cell suspension of mouse leukocytes by traditional methods or by following the instructions outlined in the Cell Preparation section of this insert. Cells must be suspended in cold 1X MagCelect Buffer prior to beginning the procedure and be at a cell density of 2×10^8 cells/mL.
3. Transfer 2×10^8 cells (1 mL volume) into a 5 mL polystyrene tube and then add 200 μL of Mouse CD3⁺ T Cell Biotinylated Antibody Cocktail. Gently mix the cell-antibody suspension, avoiding bubble formation, and incubate at 2-8 °C in a refrigerator for 15 minutes.
4. Add 200 μL of Streptavidin Ferrofluid to the cell suspension, mix gently and incubate for 15 minutes in a refrigerator at 2-8 °C.
5. At the end of the incubation period bring the volume of the reaction in the tube to 3 mL by adding 1.6 mL of 1X MagCelect Buffer. Mix gently to ensure that all reactants in the tube are in suspension.
6. Place the reaction tube in the MagCelect Magnet that has been positioned horizontally to accommodate 5 mL tubes and incubate for 6 minutes at room temperature. Magnetically tagged cells will migrate toward the magnet (these are the unwanted cells), leaving the untouched desired cells in suspension in the supernatant.
7. Recovery of desired cells is achieved as follows: While the tube is in the magnet, use a sterile Pasteur pipette or transfer pipette to carefully aspirate all of the reaction supernatant and place it in a new 5 mL tube. Remove the tube containing the magnetically trapped cells from the magnet, and discard.
8. To ensure that all of the magnetic nanoparticles have been removed, repeat the magnetic depletion (steps 6 and 7) with the new tube containing the recovered cells. The supernatant obtained at the end of these steps is the final depleted cell fraction containing the desired enriched CD3⁺ T cells. The cells are now ready for counting and further downstream applications.

TECHNICAL HINTS

- If sterile cells are required following the cell selection, the entire procedure should be carried out in a laminar flow hood to maintain sterile conditions. Use sterile equipment when pipetting reagents that will be reused at a later date.
- Avoid antibody capping on cell surfaces and non-specific cell tagging by working fast, keeping cells and solutions cold through the use of pre-cooled solutions and by adhering to the incubation times and temperatures specified in the protocol. Increased temperature and prolonged incubation times may lead to non-specific cell labeling thus lowering cell purity and yield.
- When processing different numbers of cells observe the following guidelines: keep antibody cocktail and ferrofluid incubation times and temperatures the same; keep the cell density at 2×10^8 cells/mL; add 10 μ L of the antibody cocktail per 1×10^7 cells being processed; add 10 μ L of Streptavidin Ferrofluid per 1×10^7 cells being processed.
- When processing 2×10^8 cells or fewer, use the 12 x 75 mm (5 mL) tubes with the MagCollect Magnet horizontally positioned to accommodate up to six 5 mL tubes. **Do not process more than 2×10^8 cells in each 5 mL tube and do not exceed a total reaction volume of 3 mL in each tube.** A reaction volume of 2 mL is recommended for processing 1×10^8 cells. A reaction volume of 1 mL is recommended when processing 5×10^7 or fewer cells. **Reaction volume adjustments must be made using 1X MagCollect Buffer just prior to the magnetic separation step.**
- When processing greater than 2×10^8 cells, use the 17 x 100 mm (15 mL) tubes with the MagCollect magnet vertically positioned to accommodate up to two 15 mL tubes. **Do not process more than 6×10^8 cells in each 15 mL tube and do not exceed a total reaction volume of 9 mL in each tube.** When using this larger tube, increase the reaction volume before the magnetic separation step according to the following formula: 3 mL for each 2×10^8 cells processed. Also increase the incubation time in the magnet described in step #6 to 8 minutes. **Reaction volume adjustments must be made using 1X MagCollect Buffer just prior to the magnetic separation step.**
- Sample quality can impact purity. If purity is low, the following steps might be helpful: Repeat the wash and magnetic selection step in the procedure, and/or increase the amount of ferrofluid to 1.25-fold. Decrease the volume of 1X buffer accordingly.
Note: Cell yields may be impacted.

DATA EXAMPLES

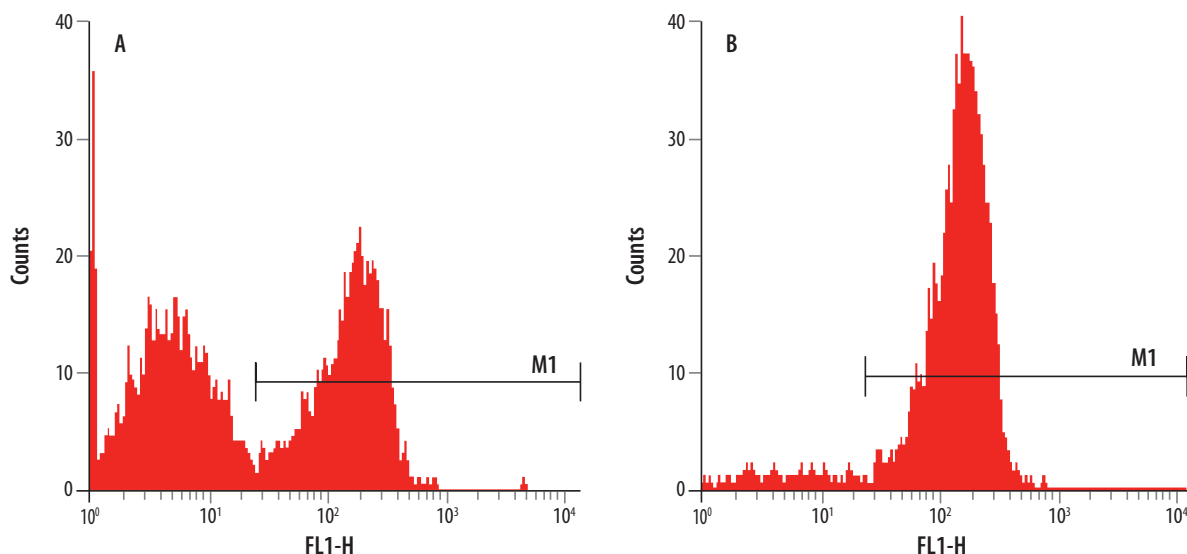

Mouse splenocytes before (A) and after (B) isolation of CD3⁺ T cells using the MagCollect Mouse CD3⁺ T Cell Isolation Kit. Histograms reflect all viable cells stained with CD3-FITC. Purity of isolated cells for this experiment was 97.5%.