

# Quantikine<sup>®</sup> ELISA

## Mouse EGFR Immunoassay

Catalog Number MEGFR0

For the quantitative determination of mouse Epidermal Growth Factor Receptor (EGFR) concentrations in cell culture supernates, serum, plasma, and urine.

This package insert must be read in its entirety before using this product.  
For research use only. Not for use in diagnostic procedures.

# TABLE OF CONTENTS

SECTION	PAGE
INTRODUCTION .....	1
PRINCIPLE OF THE ASSAY.....	2
LIMITATIONS OF THE PROCEDURE .....	2
TECHNICAL HINTS.....	2
MATERIALS PROVIDED & STORAGE CONDITIONS .....	3
OTHER SUPPLIES REQUIRED .....	3
PRECAUTIONS.....	4
SAMPLE COLLECTION & STORAGE.....	4
SAMPLE PREPARATION.....	4
REAGENT PREPARATION .....	5
ASSAY PROCEDURE .....	6
CALCULATION OF RESULTS.....	7
TYPICAL DATA.....	7
PRECISION .....	8
RECOVERY.....	8
LINEARITY.....	8
SENSITIVITY .....	9
CALIBRATION .....	9
SAMPLE VALUES.....	9
SPECIFICITY.....	10
REFERENCES.....	11
PLATE LAYOUT .....	12

## MANUFACTURED AND DISTRIBUTED BY:

### USA & Canada | R&D Systems, Inc.

614 McKinley Place NE, Minneapolis, MN 55413, USA  
TEL: (800) 343-7475 (612) 379-2956 FAX: (612) 656-4400  
E-MAIL: info@RnDSystems.com

## DISTRIBUTED BY:

### UK & Europe | R&D Systems Europe, Ltd.

19 Barton Lane, Abingdon Science Park, Abingdon OX14 3NB, UK  
TEL: +44 (0)1235 529449 FAX: +44 (0)1235 533420  
E-MAIL: info@RnDSystems.co.uk

### China | R&D Systems China Co., Ltd.

24A1 Hua Min Empire Plaza, 726 West Yan An Road, Shanghai PRC 200050  
TEL: +86 (21) 52380373 FAX: +86 (21) 52371001  
E-MAIL: info@RnDSystemsChina.com.cn

## INTRODUCTION

The Epidermal Growth Factor Receptor (EGFR), also known as Her1, ErbB1, and ErbB, is a member of the EGFR subfamily of receptor tyrosine kinases (RTKs). The EGFR family also includes ErbB2 (Neu, Her-2), ErbB3 (Her3), and ErbB4 (Her4) (1). The mature EGFR is a 170 kDa type 1 transmembrane glycoprotein that contains a 623 amino acid (aa) ligand-binding extracellular domain (ECD), a 23 aa short transmembrane domain, and a 540 aa intracellular cytoplasmic tail. The ECD is responsible for ligand binding and subsequent receptor dimerization. Within the ECD, mouse EGFR shares 88% and 93% aa sequence identity with human and rat EGFR, respectively. It shares 44-48% aa sequence identity with the ECD of mouse ErbB2, ErbB3, and ErbB4. EGFR is widely expressed on epithelial cells, predominantly in the gastrointestinal tract and breast, and is required for epithelial cell development and proliferation (2-4).

EGFR serves as the receptor for a subset of EGF family members, including EGF, TGF- $\alpha$ , HB-EGF, Amphiregulin, Betacellulin, Epiregulin, and Epigen (5, 6). These molecules are expressed as transmembrane proteins but are shed from the cell surface by proteolytic cleavage (7). Ligand binding induces EGFR homodimerization as well as heterodimerization with ErbB2, ErbB3, or ErbB4. Dimerization results in the activation of cytoplasmic kinase domains, tyrosine autophosphorylation, and internalization of the receptor-ligand complex (8, 9). Signaling through EGFR influences cell proliferation, motility, survival, and differentiation (1-4). Alterations in the structure, expression, and signaling of EGFR are involved in the metastasis of a wide variety of cancers, particularly those of epithelial origin (10, 11). Overexpression of the receptor is often found in advanced-stage carcinomas and correlates with a poor clinical prognosis (12, 13).

Soluble EGFR isoforms can be generated by alternative splicing or proteolytic cleavage. Soluble ECD fragments of 60 kDa, 80 kDa, and 110 kDa retain ligand binding capability and can dimerize with membrane bound EGFR to inhibit tyrosine kinase activity (14-17). Levels of EGFR have been found to be elevated in the serum of patients with skin, cervical, ovarian, breast, or colorectal cancer (18-21). Serum EGFR elevation is also associated with responsiveness to chemotherapy in advanced colorectal cancer (21). In contrast, serum EGFR is reduced in ovarian carcinoma, non-small cell lung cancer, and head and neck carcinoma (22, 23). A decrease of serum EGFR relative to soluble ErbB2 is associated with decreased life expectancy in patients with metastatic breast cancer (24). Evidence linking EGFR, tumorigenesis, and cancer progression has instigated clinical use of targeted treatments against the receptor and its signaling components (25).

The Quantikine<sup>®</sup> Mouse EGFR Immunoassay is a 4.5 hour solid phase ELISA designed to measure mouse EGFR levels in cell culture supernates, serum, plasma, and urine. It contains NS0-expressed recombinant mouse EGFR and antibodies raised against the recombinant factor. This immunoassay has been shown to quantitate the recombinant mouse EGFR accurately. Results obtained using natural mouse EGFR showed dose-response curves that were parallel to the standard curves obtained using the Quantikine<sup>®</sup> kit standards. These results indicate that this kit can be used to determine relative mass values for natural mouse EGFR.

## PRINCIPLE OF THE ASSAY

This assay employs the quantitative sandwich enzyme immunoassay technique. A monoclonal antibody specific for mouse EGFR has been pre-coated onto a microplate. Standards, control, and samples are pipetted into the wells and any EGFR present is bound by the immobilized antibody. After washing away any unbound substances, an enzyme-linked polyclonal antibody specific for mouse EGFR is added to the wells. Following a wash to remove any unbound antibody-enzyme reagent, a substrate solution is added to the wells. The enzyme reaction yields a blue product that turns yellow when the Stop Solution is added. The intensity of the color measured is in proportion to the amount of EGFR bound in the initial step. The sample values are then read off the standard curve.

## LIMITATIONS OF THE PROCEDURE

- FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.
- The kit should not be used beyond the expiration date on the kit label.
- Do not mix or substitute reagents with those from other lots or sources.
- Samples, controls, and standards must be pipetted within 15 minutes.
- If samples generate values higher than the highest standard, further dilute the samples with calibrator diluent and repeat the assay.
- Any variation in diluent, operator, pipetting technique, washing technique, incubation time or temperature, and kit age can cause variation in binding.
- Variations in sample collection, processing, and storage may cause sample value differences.
- This assay is designed to eliminate interference by other factors present in biological samples. Until all factors have been tested in the Quantikine® Immunoassay, the possibility of interference cannot be excluded.

## TECHNICAL HINTS

- When mixing or reconstituting protein solutions, always avoid foaming.
- To avoid cross-contamination, change pipette tips between additions of each standard level, between sample additions, and between reagent additions. Also, use separate reservoirs for each reagent.
- To ensure accurate results, proper adhesion of plate sealers during incubation steps is necessary.
- Substrate Solution should remain colorless until added to the plate. Keep Substrate Solution protected from light. Substrate Solution should change from colorless to gradations of blue.
- Stop Solution should be added to the plate in the same order as the Substrate Solution. The color developed in the wells will turn from blue to yellow upon addition of the Stop Solution.

## MATERIALS PROVIDED & STORAGE CONDITIONS

Store the unopened kit at 2-8 °C. Do not use past kit expiration date.

PART	PART #	DESCRIPTION	STORAGE OF OPENED/ RECONSTITUTED MATERIAL
Mouse EGFR Microplate	894740	96 well polystyrene microplate (12 strips of 8 wells) coated with a monoclonal antibody specific for mouse EGFR.	Return unused wells to the foil pouch containing the desiccant pack. Reseal along entire edge of the zip-seal. May be stored for up to 1 month at 2-8 °C.*
Mouse EGFR Standard	894742	2 vials of recombinant mouse EGFR in a buffered protein base with preservatives; lyophilized. <i>Refer to the vial label for reconstitution volume.</i>	Use a new standard and control for each assay. Discard after use.
Mouse EGFR Control	894743	2 vials of recombinant mouse EGFR in a buffered protein base with preservatives; lyophilized. The assay value of the control should be within the range specified on the label.	
Mouse EGFR Conjugate	894741	12 mL of a polyclonal antibody specific for mouse EGFR conjugated to horseradish peroxidase with preservatives.	May be stored for up to 1 month at 2-8 °C.*
Assay Diluent RD1-34	895265	11 mL of a buffer with blue dye and preservatives.	
Calibrator Diluent RD5P	895151	21 mL of a concentrated buffered protein base with preservatives. <i>Use diluted 1:5 in this assay.</i>	
Wash Buffer Concentrate	895003	21 mL of a 25-fold concentrated solution of buffered surfactant with preservative. <i>May turn yellow over time.</i>	
Color Reagent A	895000	12 mL of stabilized hydrogen peroxide.	
Color Reagent B	895001	12 mL of stabilized chromogen (tetramethylbenzidine).	
Stop Solution	895174	23 mL of diluted hydrochloric acid.	
Plate Sealers	N/A	4 adhesive strips.	

\* Provided this is within the expiration date of the kit.

## OTHER SUPPLIES REQUIRED

- Microplate reader capable of measuring absorbance at 450 nm, with the correction wavelength set at 540 nm or 570 nm.
- Pipettes and pipette tips.
- Deionized or distilled water.
- Squirt bottle, manifold dispenser, or automated microplate washer.
- 100 mL and 500 mL graduated cylinders.
- Test tubes for dilution of standards and samples.

## PRECAUTIONS

The Stop Solution provided with this kit is an acid solution.

Some components in this kit contain a preservative which may cause an allergic skin reaction. Avoid breathing mist.

Color Reagent B may cause skin, eye, and respiratory irritation. Avoid breathing fumes.

Wear protective gloves, clothing, eye, and face protection. Wash hands thoroughly after handling. Refer to the MSDS on our website prior to use.

## SAMPLE COLLECTION & STORAGE

**The sample collection and storage conditions listed below are intended as general guidelines. Sample stability has not been evaluated.**

**Cell Culture Supernates** - Remove particulates by centrifugation. Assay immediately or aliquot and store samples at  $\leq -20$  °C. Avoid repeated freeze-thaw cycles.

**Serum** - Allow blood samples to clot for 2 hours at room temperature before centrifuging for 20 minutes at 2000 x g. Remove serum and assay immediately or aliquot and store samples at  $\leq -20$  °C. Avoid repeated freeze-thaw cycles.

**Plasma** - Collect plasma using EDTA or heparin as an anticoagulant. Centrifuge for 20 minutes at 2000 x g within 30 minutes of collection. Assay immediately or aliquot and store samples at  $\leq -20$  °C. Avoid repeated freeze-thaw cycles.

**Note:** *Citrate plasma has not been validated for use in this assay.  
Grossly hemolyzed samples are not suitable for use in this assay.*

**Urine** - Collect urine using a metabolic cage. Remove any particulates by centrifugation and assay immediately or aliquot and store samples at  $\leq -20$  °C. Avoid repeated freeze-thaw cycles. Centrifuge again before assaying to remove any additional precipitates that may appear after storage.

## SAMPLE PREPARATION

Serum and plasma samples require a 500-fold dilution due to high endogenous values. A suggested 500-fold dilution can be achieved by adding 10  $\mu$ L of sample to 490  $\mu$ L of Calibrator Diluent RD5P (diluted 1:5)\*. Complete the 500-fold dilution by adding 50  $\mu$ L of the diluted sample to 450  $\mu$ L Calibrator Diluent RD5P (diluted 1:5)\*.

Urine samples require an 8-fold dilution due to matrix effects. A suggested 8-fold dilution is 20  $\mu$ L of sample + 140  $\mu$ L of Calibrator Diluent RD5P (diluted 1:5)\*.

\*See Reagent Preparation section

## REAGENT PREPARATION

**Bring all reagents to room temperature before use.**

**Mouse EGFR Control** - Reconstitute the control with 1.0 mL of deionized or distilled water. Mix thoroughly. Assay the control undiluted.


**Wash Buffer** - If crystals have formed in the concentrate, warm to room temperature and mix gently until the crystals have completely dissolved. Add 20 mL of Wash Buffer Concentrate to deionized or distilled water to prepare 500 mL of Wash Buffer.

**Calibrator Diluent RD5P (diluted 1:5)** - Add 20 mL of Calibrator Diluent RD5P to 80 mL of deionized or distilled water to prepare 100 mL of Calibrator Diluent RD5P (diluted 1:5).

**Substrate Solution** - Color Reagents A and B should be mixed together in equal volumes within 15 minutes of use. Protect from light. 100  $\mu$ L of the resultant mixture is required per well.

**Mouse EGFR Standard - Refer to the vial label for reconstitution volume.** Reconstitute the Mouse EGFR Standard with Calibrator Diluent RD5P (diluted 1:5). This reconstitution produces a stock solution of 30 ng/mL. Allow the standard to sit for a minimum of 5 minutes with gentle mixing prior to making dilutions.

Pipette 300  $\mu$ L of Calibrator Diluent RD5P (diluted 1:5) into each tube. Use the stock solution to produce a dilution series (below). Mix each tube thoroughly before the next transfer. The undiluted Mouse EGFR Standard (30 ng/mL) serves as the high standard. Calibrator Diluent RD5P (diluted 1:5) serves as the zero standard (0 ng/mL).

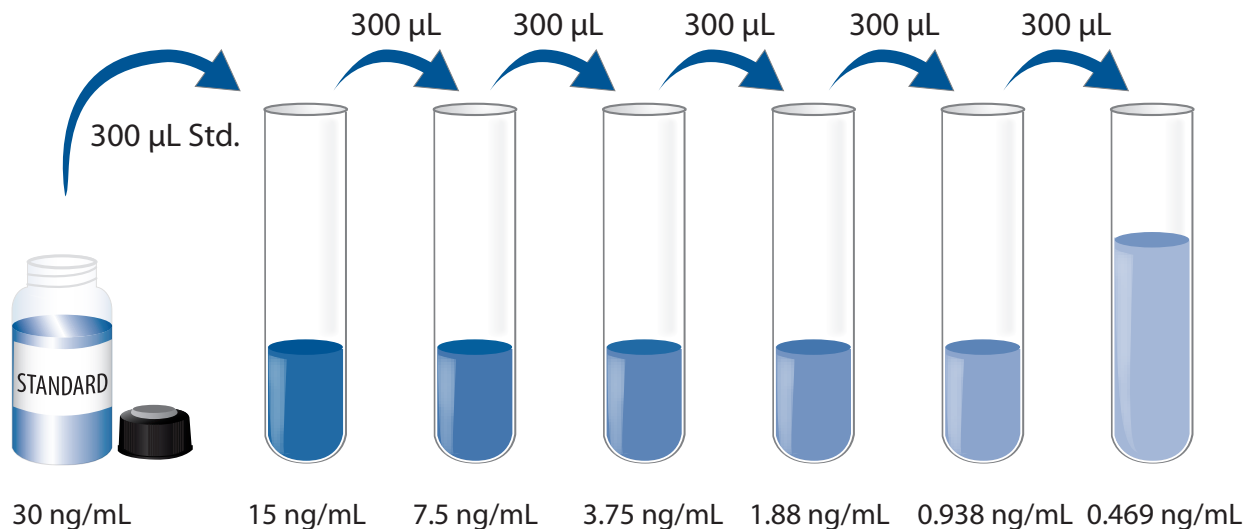

## ASSAY PROCEDURE

**Bring all reagents and samples to room temperature before use. It is recommended that all standards, control, and samples be assayed in duplicate.**

1. Prepare all reagents, working standards, control, and samples as directed in the previous sections.
2. Remove excess microplate strips from the plate frame, return them to the foil pouch containing the desiccant pack, and reseal.
3. Add 50  $\mu$ L of Assay Diluent RD1-34 to each well.
4. Add 50  $\mu$ L of standard, control, or sample\* per well. Cover with the adhesive strip provided. Incubate for 2 hours at room temperature. A plate layout is provided to record standards and samples assayed.

**Note:** *Samples, controls, and standards must be pipetted within 15 minutes.*

5. Aspirate each well and wash, repeating the process three times for a total of four washes. Wash by filling each well with Wash Buffer (400  $\mu$ L) using a squirt bottle, manifold dispenser, or autowasher. Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels.
6. Add 100  $\mu$ L of Mouse EGFR Conjugate to each well. Cover with a new adhesive strip. Incubate for 2 hours at room temperature.
7. Repeat the aspiration/wash as in step 4.
8. Add 100  $\mu$ L of Substrate Solution to each well. Incubate for 30 minutes at room temperature on the benchtop. **Protect from light.**
9. Add 100  $\mu$ L of Stop Solution to each well. Gently tap the plate to ensure thorough mixing.
10. Determine the optical density of each well within 30 minutes, using a microplate reader set to 450 nm. If wavelength correction is available, set to 540 nm or 570 nm. If wavelength correction is not available, subtract readings at 540 nm or 570 nm from the readings at 450 nm. This subtraction will correct for optical imperfections in the plate. Readings made directly at 450 nm without correction may be higher and less accurate.

\*Samples may require dilution. See Sample Preparation section.



## CALCULATION OF RESULTS


Average the duplicate readings for each standard, control, and sample and subtract the average zero standard optical density (O.D.).

Create a standard curve by reducing the data using computer software capable of generating a four parameter logistic (4-PL) curve-fit. As an alternative, construct a standard curve by plotting the mean absorbance for each standard on the y-axis against the concentration on the x-axis and draw a best fit curve through the points on the graph. The data may be linearized by plotting the log of the mouse EGFR concentrations versus the log of the O.D. and the best fit line can be determined by regression analysis. This procedure will produce an adequate but less precise fit of the data.

If samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.

## TYPICAL DATA

This standard curve is provided for demonstration only. A standard curve should be generated for each set of samples assayed.

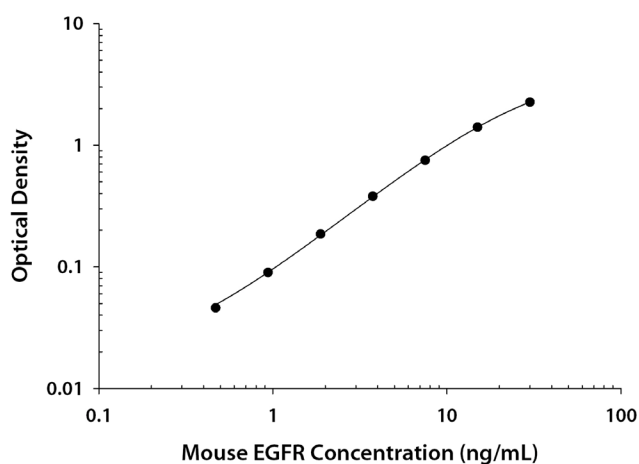

(ng/mL)	O.D.	Average	Corrected
0	0.011 0.013	0.012	—
0.469	0.056 0.059	0.058	0.046
0.938	0.098 0.105	0.102	0.090
1.88	0.198 0.198	0.198	0.186
3.75	0.383 0.400	0.392	0.380
7.5	0.742 0.783	0.763	0.751
15	1.405 1.435	1.420	1.408
30	2.241 2.301	2.271	2.259

## PRECISION

### Intra-assay Precision (Precision within an assay)

Three samples of known concentration were tested twenty times on one plate to assess intra-assay precision.

### Inter-assay Precision (Precision between assays)

Three samples of known concentration were tested in twenty separate assays to assess inter-assay precision. Assays were performed by at least three technicians using two lots of components.

Sample	Intra-Assay Precision			Inter-Assay Precision		
	1	2	3	1	2	3
n	20	20	20	20	20	20
Mean (ng/mL)	1.11	2.58	5.41	0.976	2.42	5.13
Standard deviation	0.049	0.080	0.159	0.090	0.114	0.197
CV (%)	4.4	3.1	2.9	9.2	4.7	3.8

## RECOVERY

The recovery of mouse EGFR spiked to three levels throughout the range of the assay in various matrices was evaluated.

Sample Type	Average % Recovery	Range
Cell culture media (n=4)	103	94-107%
Urine* (n=4)	86	79-94%

\*Samples were diluted prior to assay as directed in the Sample Preparation section.

## LINEARITY

To assess the linearity of the assay, samples containing and/or spiked with high concentrations of mouse EGFR were serially diluted with calibrator diluent to produce samples with values within the dynamic range of the assay.

		Cell culture media (n=4)	Serum* (n=4)	EDTA plasma* (n=4)	Heparin plasma* (n=4)	Urine* (n=4)
1:2	Average % of Expected	97	100	102	101	105
	Range (%)	94-99	98-103	100-105	99-104	103-107
1:4	Average % of Expected	96	103	103	103	109
	Range (%)	94-98	97-107	101-106	100-106	104-112
1:8	Average % of Expected	96	108	104	104	114
	Range (%)	94-99	98-114	103-107	101-108	103-123
1:16	Average % of Expected	96	108	109	108	117
	Range (%)	94-100	97-115	105-112	102-114	104-126

\*Samples were diluted prior to assay as directed in the Sample Preparation section.

## SENSITIVITY

Thirty assays were evaluated and the minimum detectable dose (MDD) of mouse EGFR ranged from 0.016-0.127 ng/mL. The mean MDD was 0.038 ng/mL.

The MDD was determined by adding two standard deviations to the mean O.D. value of twenty zero standard replicates and calculating the corresponding concentration.

## CALIBRATION

This immunoassay is calibrated against a highly purified NS0-derived recombinant mouse EGFR produced at R&D Systems®.

## SAMPLE VALUES

**Serum/Plasma/Urine** - Samples were evaluated for the presence of mouse EGFR in this assay.

Sample Type	Mean (ng/mL)	Range (ng/mL)	Standard Deviation (ng/mL)
Serum (n=10)	7118	3008-15,839	3689
EDTA plasma (n=5)	7909	3522-14,214	4934
Heparin plasma (n=5)	8514	2711-11,384	3520
Urine (n=5)	23.3	12.7-41.7	11.1

**Cell Culture Supernates** - Organs from mice were removed, rinsed in PBS, and kept on ice. The organs were then homogenized using a tissue homogenizer and cultured in RPMI 1640 supplemented with 10% fetal bovine serum, 2 mM L-glutamine, 100 U/mL penicillin, and 100 µg/mL streptomycin sulfate for 2 days. Aliquots of the cell culture supernates were removed and assayed for levels of mouse EGFR.

Tissue Type	(ng/mL)
Brain	0.753
Liver	9.13

## SPECIFICITY

This assay recognizes natural and recombinant mouse EGFR.



The factors listed below were prepared in 300 ng/mL of calibrator diluent and assayed for cross-reactivity. Preparations of the following factors in 300 ng/mL of a mid-range recombinant mouse EGFR control were assayed for interference. No significant cross-reactivity or interference was observed.

### Recombinant mouse:

Amphiregulin  
Betacellulin  
EGF  
EGF (pro)  
Epigen  
Epiregulin  
ErbB2  
ErbB3  
ErbB4  
HB-EGF

### Recombinant human:

EGF  
EGF (pro)  
EGFR  
Epigen  
HB-EGF  
TGF- $\alpha$

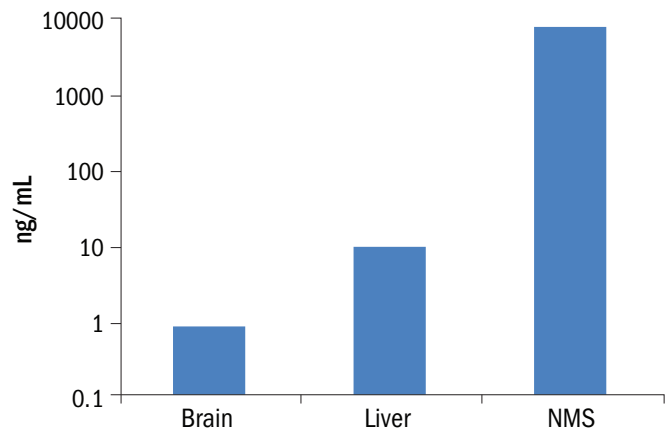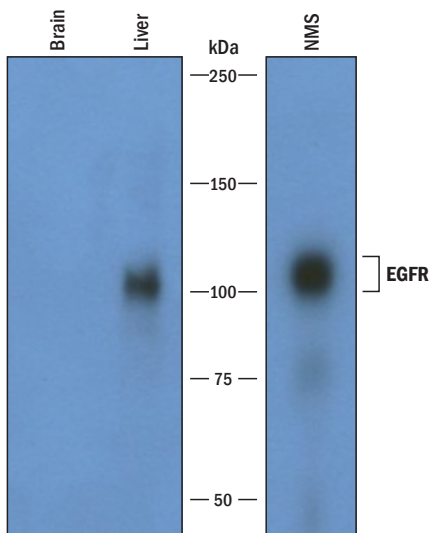

Conditioned media from mouse brain, liver, and normal mouse serum (NMS) samples were analyzed by Western Blot and Quantikine<sup>®</sup> ELISA. The Conditioned media and serum samples were resolved under reducing SDS-PAGE conditions, transferred to a PVDF membrane, and immunoblotted with the detection antibody in this kit. The Western Blot shows a direct correlation with the ELISA value for these samples.

## REFERENCES

1. Singh, A.B. and R.C. Harris (2005) *Cell Signal.* **17**:1183.
2. Miettinen, P.J. *et al.* (1995) *Nature* **376**:337.
3. Real, F.X. *et al.* (1986) *Cancer Res.* **46**:4726.
4. Sibia, M. and E.F. Wagner (1995) *Science* **269**:234.
5. Harris, R.C. *et al.* (2003) *Exp. Cell. Res.* **284**:2.
6. Higashiyama, S. *et al.* (2008) *Cancer Sci.* **99**:214.
7. Schlessinger, J. (2002) *Cell* **110**:669.
8. Lemmon, M.A. *et al.* (1997) *EMBO J.* **16**:281.
9. Yarden, Y. and J. Schlessinger (1987) *Biochemistry* **26**:1434.
10. Citri, A. and Y. Yarden (2006) *Nat. Rev. Mol. Cell Biol.* **7**:505.
11. Rowinsky, E.K. (2004) *Annu. Rev. Med.* **55**:433.
12. Oh, M.J. *et al.* (2000) *Clin. Cancer Res.* **6**:4760.
13. Ohsaki, Y. *et al.* (2000) *Oncol. Rep.* **7**:603.
14. Reiter, J.L. *et al.* (2001) *Genomics* **71**:1.
15. Guillaudeau, A. *et al.* (2012) *PLoS One* **7**:e37204.
16. Perez-Torres, M. *et al.* (2008) *Exp. Cell Res.* **314**:2907.
17. Sanderson, M.P. *et al.* (2008) *J. Cell Biochem.* **103**:1783.
18. Kanemura, H. *et al.* (2013) *Clin. Exp. Dermatol.* **38**:172.
19. Lee, M.Y. *et al.* (2008) *Clin. Cancer Res.* **14**:4743.
20. Baron, A.T. *et al.* (2009) *Cancer Treat. Res.* **149**:189.
21. Zampino, M.G. *et al.* (2008) *Cancer Chemother. Pharmacol.* **63**:139.
22. Baron, A.T. *et al.* (2003) *Cancer Epidemiol. Biomarkers Prev.* **12**:103.
23. Lemos-Gonzalez, Y. *et al.* (2007) *Br. J. Cancer* **96**:1569.
24. Souder, C. *et al.* (2006) *Cancer* **107**:2337.
25. Peipp, M. *et al.* (2009) *MAbs* **1**:590.

**PLATE LAYOUT**

Use this plate layout to record standards and samples assayed.

12									
11									
10									
9									
8									
7									
6									
5									
4									
3									
2									
1									
	A	B	C	D	E	F	G	H	

**NOTES**

**NOTES**

*All trademarks and registered trademarks are the property of their respective owners.*

©2017 R&D Systems®, Inc.