PRODUCT INFORMATION & MANUAL

Human IL-2 Valukine™ ELISA

Catalog Number: VAL110

For the quantitative determination of natural and recombinant human Interleukin 2 (IL-2) concentrations

For research use only.
Not for diagnostic or therapeutic procedures.

Bio-Techne China Co. Ltd
P: +86 (21) 52380373 P: 8009881270 F: +86 (21) 52381001
info.cn@bio-techne.com

Please refer to the kit label for expiry date.
Novus kits are guaranteed for 3 months from date of receipt

Version 202605.6

TABLE OF CONTENTS

I. BACKGROUND 2

II. OVERVIEW 3

III. ADVANTAGES 4

IV. EXPERIMENT 8

V. KIT COMPONENTS AND STORAGE 9

VI. PREPARATION 12

VII. ASSAY PROCEDURE 14

VIII. REFERENCES 16

I. BACKGROUND

Human Interleukin 2 (IL-2), also known as T cell growth factor (TCGF), is a 15-18 kDa variably glycosylated α-helical polypeptide that is a member of the common gamma chain (γc) cytokine family (1-4). It exists as a monomer and has a notably short half-life (<30 minutes) (1). Human IL-2 is synthesized as a 153 amino acid (aa) precursor that contains a 20 aa signal sequence plus a 133 aa mature region (5, 6). The mature region contains one utilized O-linked glycosylation site at Thr3, plus three cysteines, two of which form an intrachain disulfide bond that is essential for activity (7). Mature human IL-2 shares 73%, 66%, 78% and 97% aa sequence identity with canine, rat, feline and rhesus monkey IL-2, respectively. Although human IL-2 shares only approximately 60% aa identify with the highly polymorphic mouse IL-2, human IL-2 is known to be active on mouse IL-2 responsive cells. Cells reported to secrete IL-2 include γδ T cells (8), activated conventional $CD4^+$ and $CD8^+$ T cells (1, 9), neurons (10, 11), microglia (12), and hematopoietic stem cells (13).

The receptor for IL-2 (IL-2R) is composed of three subunits, the 55 kDa CD25/IL-2Rα chain, the 70 kDa CD122/IL-2Rβ chain, and the 65 kDa CD132/ γc chain (1, 3). IL-2 first binds to CD25, the binary complex then recruits CD122 and CD132 to form the quaternary signaling complex (1, 14). In addition to IL-2, CD122/IL-2Rβ is used by IL-15 in its quaternary signaling complex. CD132/ γc also serves as a signaling receptor for IL-4, -7, -9, -15 and -21 (1, 3).

In vitro studies have shown an important role for IL-2 in T cell activation and expansion. In vivo, IL-2 is critical for the development, maintenance and function of regulatory T cells (Treg) which provide protection against autoimmune disease. On the other hand, IL-2 can also promote autoimmune inflammation in target organs through its roles in regulating the expression of T cell trafficking genes, and production of Th2 cytokines. Within the $CD8^+$ T cell subset, IL-2 is essential for optimal primary responses and differentiation into terminal effector cells. IL-2 also promotes the development of activated $CD8^+$ T cells into memory cells (1).

II. OVERVIEW

A. PRINCIPLE OF THE ASSAY

This assay employs the quantitative sandwich enzyme immunoassay technique. An antibody specific for human IL-2 has been pre-coated onto a microplate. Standards and samples are pipetted into the wells and any human IL-2 present is bound by the immobilized antibody. After washing away any unbound substances, an enzyme-linked antibody specific for human IL-2 is added to the wells. Following a wash to remove any unbound antibody-enzyme reagent, TMB substrate (Chromogenic agent) is added to the wells and color develops in proportion to the amount of human IL-2 bound in the initial step. The color development is stopped, and the intensity of the color is measured.

B. LIMITATIONS OF THE PROCEDURE

- **FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.**
- This kit is suitable for cell culture supernate and human serum, human plasma.
- The kit should not be used beyond the expiration date on the kit label.
- Do not mix or substitute reagents with those from other lots or sources.
- If samples generate values higher than the highest standard, dilute the samples with Calibrator Diluent RD5-5/RD6E and repeat the assay.
- Any variation in operator, pipetting technique, washing technique, incubation time or temperature, and kit age can cause variation in binding.

III. ADVANTAGES

A. PRECISION

Intra-assay Precision (Precision within an assay)

Three samples were tested twenty times on one plate to assess intra-assay precision.

Inter-assay Precision (Precision between assays)

Three samples were tested in twenty separate assays to assess inter-assay precision.

CELL CULTURE SUPERNATE ASSAY

	Intra-assay Precision			**Inter-assay Precision**		
Sample	1	2	3	1	2	3
Mean (pg/mL)	67.5	438	851	232	620	1148
Standard Deviation	2.9	14.4	26.9	23.2	34.4	45.5
CV%	4.3	3.3	3.2	10.0	5.5	4.0

SERUM/PLASMA ASSAY

	Intra-assay Precision			**Inter-assay Precision**		
Sample	1	2	3	1	2	3
Mean (pg/mL)	98.0	619	1183	250	755	1470
Standard Deviation	4.2	18.0	24.0	12.6	27.8	74.1
CV%	4.3	2.9	2.0	5.0	3.7	5.0

B. RECOVERY

The recovery of human IL-2 spiked to three levels in samples throughout the range of the assay was evaluated.

Sample Type	Average % Recovery	Range (%)
Cell culture media (n=5)	101	96 - 107
Serum (n=5)	99	89 - 114
EDTA plasma (n=5)	118	104 - 139
Heparin plasma (n=5)	109	94 - 129
Citrate plasma (n=5)	105	98 - 111

C. SENSITIVITY

The minimum detectable dose (MDD) of IL-2 is typically less than 7 pg/mL.

The MDD was determined by adding two standard deviations to the mean optical density value of twenty zero standard replicates and calculating the corresponding concentration.

D. CALIBRATION

This immunoassay is calibrated against highly purified *E. coli*-expressed recombinant human IL-2 produced at R&D Systems®.

NIBSC/WHO 1st International natural human IL-2 Standard 86/504, which was intended as a potency standard, the non-WHO interim reference recombinant human IL-2 Standard 86/564, and the 2nd International Standard recombinant human IL-2 86/500 were evaluated in this kit. All materials parallel the Valukine® Human IL-2 standard curve. To convert sample values obtained with the Valukine® Human IL-2 kit to relative approximate NIBSC units, use the appropriate equation below:

NIBSC (86/500) approximate value (IU/mL) = 0.017 x Valukine® Human IL-2 value (pg/mL)

NIBSC (86/504) approximate value (IU/mL) = 0.016 x Valukine® Human IL-2 value (pg/mL)

NIBSC (86/564) approximate value (U/mL) = 0.012 x Valukine® Human IL-2 value (pg/mL)

Note: *Based on data generated in September 2008*.

E. LINEARITY

To assess the linearity of the assay, different samples were containing or spiked with high concentrations of human IL-2 in various matrices and diluted with the appropriate Calibrator Diluent RD5-5/RD6E to produce samples with values within the dynamic range of the assay.

		Cell culture media (n=5)	**Serum (n=5)**	**EDTA plasma (n=5)**	**Heparin plasma (n=5)**	**Citrate plasma (n=5)**
1:2	Average % of Expected	102	97	100	104	100
	Range (%)	90 - 113	95 - 102	89 - 106	100 - 109	96 - 105
1:4	Average % of Expected	101	94	102	104	99
	Range (%)	90 - 111	91 - 97	97 - 107	99 - 108	96 - 102
1:8	Average % of Expected	99	87	99	100	97
	Range (%)	91 - 108	78 - 92	92 - 106	94 - 107	91 - 100
1:16	Average % of Expected	___	___	98	95	91
	Range (%)	___	___	88 - 114	86 - 109	85 - 100

F. SAMPLE VALUES

Serum/Plasma - Thirty-seven serum and plasma samples from apparently healthy volunteers were evaluated for the presence of human IL-2 in this assay. All samples measured less than the lowest Human IL-2 Standard, 31.3 pg/mL. No medical histories were available for the donors used in this study.

G. SPECIFICITY

This assay recognizes both natural and recombinant human IL-2.

The following factors were prepared at 100 ng/mL in calibrator diluent RD5-5/RD6E and assayed for cross-reactivity. Preparations of the following factors at 100 ng/mL in a mid-range recombinant human IL-2 control were assayed for interference. No significant cross-reactivity or interference was observed.


Recombinant human		**Recombinant mouse**
G-CSF	IL-6	GM-CSF
GM-CSF	IL-7	IL-1β
IL-1α	IL-8	IL-2
IL-1β	LIF	IL-3
IL-2 Rα	TGF-β1	IL-4
IL-2 Rβ	TGF-β2	IL-5
IL-2 Rγ	TNF-α	IL-6
IL-3	TNF-β	IL-7
IL-4		

IV. EXPERIMENT

EXAMPLE STANDARD


The standard curve is provided for demonstration only. A standard curve should be generated for each set of samples assayed.

CELL CULTURE SUPERNATE ASSAY

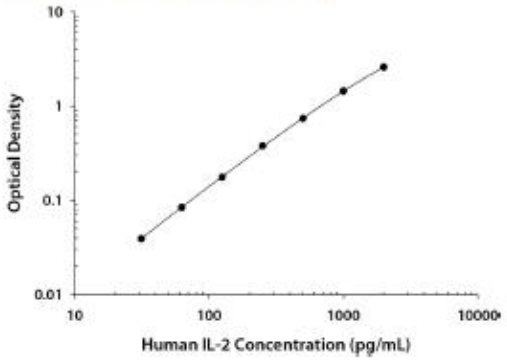

(pg/mL)	O.D.	Average	Corrected
0	0.042	0.040	——
	0.039		
31.3	0.081	0.079	0.039
	0.077		
62.5	0.127	0.124	0.084
	0.120		
125	0.221	0.216	0.176
	0.210		
250	0.404	0.418	0.378
	0.431		
500	0.802	0.779	0.739
	0.756		
1000	1.513	1.485	1.445
	1.457		
2000	2.734	2.630	2.590
	2.527		

SERUM/PLASMA ASSAY

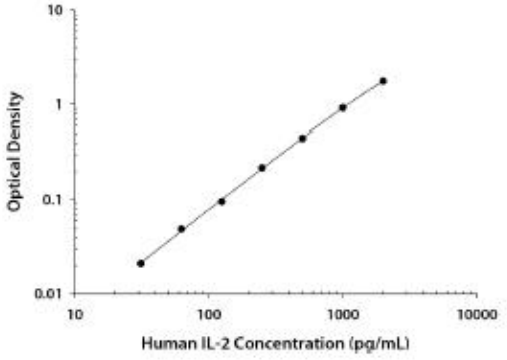

(pg/mL)	O.D.	Average	Corrected
0	0.035	0.033	——
	0.031		
31.3	0.054	0.054	0.021
	0.054		
62.5	0.084	0.082	0.049
	0.081		
125	0.121	0.129	0.096
	0.137		
250	0.247	0.252	0.219
	0.258		
500	0.474	0.482	0.449
	0.489		
1000	0.956	0.950	0.917
	0.945		
2000	1.785	1.792	1.759
	1.799		

V. KIT COMPONENTS AND STORAGE

A. MATERIALS PROVIDED

Parts	Description	Size
Human IL-2 Microplate	96 well polystyrene microplate (12 strips of 8 wells) coated with an antibody against human IL-2	1 plate
Human IL-2 Conjugate	Solution of antibody against human IL-2 conjugated to horseradish peroxidase	1 vial
Human IL-2 Standard	Recombinant human IL-2 in a buffered protein base; lyophilized. *Refer to the vial label for reconstitution volume*	1 vial
Assay Diluent RD1W	A buffered protein base with preservatives.	1 vial
Calibrator Diluent RD5-5	A buffered protein base with preservatives. *For cell culture supernate samples.*	1 vial
Calibrator Diluent RD6E	Animal serum with preservatives. *For serum/plasma samples.*	1 vial
Wash Buffer Concentrate (25×)	A 25× concentrated solution of buffered surfactant	1 vial
TMB Substrate	TMB ELISA Substrate Solution/TMB Substrate Solution	2 vials
Stop Solution	2 N sulfuric acid	1 vial
Plate Sealers	Adhesive strip	3 strips

B. STORAGE

<table>
<tr><td>Unopened Kit</td><td colspan="2">Store at 2-8°C. Do not use past kit expiration date.</td></tr>
<tr><td rowspan="8">Opened/ Reconstituted Reagents</td><td>Wash Buffer (1×)</td><td rowspan="4">May be stored for up to 1 month at 2-8°C.*</td></tr>
<tr><td>Stop Solution</td></tr>
<tr><td>Conjugate</td></tr>
<tr><td>TMB Substrate</td></tr>
<tr><td>Standard</td><td>Aliquot and store for up to 1 month at <-20°C in a manual defrost freezer. * Avoid repeated freeze-thaw cycles.</td></tr>
<tr><td>Assay Diluent RD1W</td><td rowspan="3">May be stored for up to 1 month at 2-8 °C.*</td></tr>
<tr><td>Calibrator Diluent /RD5-5</td></tr>
<tr><td>Calibrator Diluent RD6E</td></tr>
<tr><td>Microplate Wells</td><td>Return unused wells to the foil pouch containing the desiccant pack, reseal along entire edge of zip-seal. May be stored for up to 1 month at 2-8°C.*</td></tr>
</table>

* Provided this is within the expiration date of the kit.

C. OTHER SUPPLIES REQUIRED

- Microplate reader capable of measuring absorbance at 450 nm, with the correction wavelength set at 540 nm or 570 nm.
- Pipettes and pipette tips.
- Deionized or distilled water.
- Squirt bottle, manifold dispenser, or automated microplate washer.
- 500 mL graduated cylinder.

D. PRECAUTION

- Calibrator Diluent RD6E contains sodium azide, which may react with lead and copper plumbing to form explosive metallic azides. Flush with large volumes of water during disposal.
- Some components in this kit contain a preservative which may cause an allergic skin reaction. Avoid breathing mist.
- The Stop Solution provided with this kit is an acid solution. Wear eye, hand, face, and clothing protection when using this material.

VI. PREPARATION

A. SAMPLE COLLECTION AND STORAGE

The sample collection and storage conditions listed below are intended as general guidelines. Sample stability has not been evaluated.

Cell Culture Supernates - Remove particulates by centrifugation and assay immediately or aliquot and store samples at ≤-20 °C. Avoid repeated freeze-thaw cycles. Samples may require dilution with Calibrator Diluent RD5-5.

Serum - Use a serum separator tube (SST) and allow samples to clot for 30 minutes at room temperature before centrifugation for 15 minutes at 1000 × g. Remove serum and assay immediately or aliquot and store samples at ≤-20 °C. Avoid repeated freeze-thaw cycles. Samples may require dilution with Calibrator Diluent RD6E.


Plasma - Collect plasma using EDTA, heparin, or citrate as an anticoagulant. Centrifuge for 15 minutes at 1000 x g within 30 minutes of collection. Assay immediately or aliquot and store samples at ≤-20 °C. Avoid repeated freeze-thaw cycles. Samples may require dilution with Calibrator Diluent RD6E.

B. REAGENT PREPARATION

Note: Bring all reagents to room temperature before use.

Wash Buffer (1×) - If crystals have formed in the concentrate, warm to room temperature and mix gently until the crystals have completely dissolved. Dilute 20 mL of Wash Buffer Concentrate (25×) into deionized or distilled water to prepare 500 mL of Wash Buffer (1×).

Human IL-2 Standard- Refer to the vial label for the reconstitution volume Reconstitute the Human IL-2 Standard with Calibrator Diluent RD5-5 (*for cell culture supernate samples*) or Calibrator Diluent RD6E (*for serum/plasma samples*). This reconstitution produces a stock solution of 2000 pg/mL. Allow the standard to sit for a minimum of 15 minutes with gentle agitation prior to making dilutions.Pipette 500 µL of the Calibrator Diluent RD5-5 (*for cell culture supernate samples*) or Calibrator Diluent RD6E (*for serum/plasma samples*) into each tube. Use the stock solution to produce a dilution series (below). Mix each tube thoroughly before the next transfer. The undiluted Human IL-2 standard serves as the high standard (2000 pg/mL). The appropriate Calibrator Diluent RD5-5/RD6E serves as the zero standard (0 pg/mL).

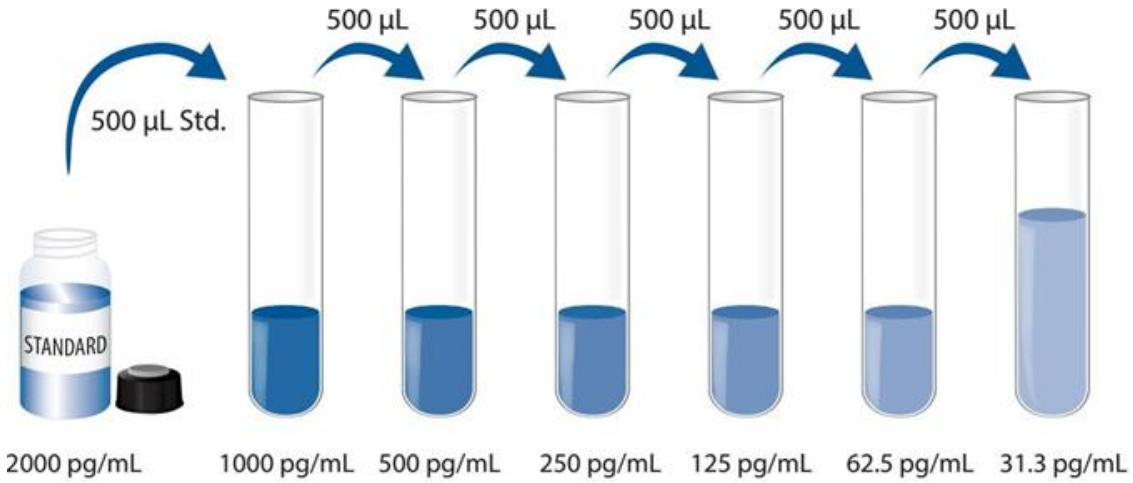

C. TECHNICAL HINTS

- When mixing or reconstituting protein solutions, always avoid foaming.
- To avoid cross-contamination, change pipette tips between additions of each standard level, between sample additions, and between reagent additions. Also, use separate reservoirs for each reagent.
- It is recommended that the samples be pipetted within 15 minutes.
- To ensure accurate results, proper adhesion of plate sealers during incubation steps is necessary.
- TMB Substrate should remain colorless until added to the plate. Keep TMB Substrate protected from light. TMB Substrate should change from colorless to gradations of blue.
- Stop Solution should be added to the plate in the same order as the TMB Substrate. The color developed in the wells will turn from blue to yellow upon addition of the Stop Solution. Wells that are green in color indicate that the Stop Solution has not mixed thoroughly with the TMB Substrate.

VII.ASSAY PROCEDURE

Note: Bring all reagents and samples to room temperature before use. It is recommended that all samples and standards be assayed in duplicate.

1. Prepare all reagents, samples and working standards as directed in the previous sections.
2. Remove excess microplate strips from the plate frame, return them to the foil pouch containing the desiccant pack, and reseal.
3. Add 100 µL of Assay Diluent RD1W to each well.
4. Add 100 µL of standard and prepared sample per well. Cover with the adhesive strip provided. **Incubate for 2 hours at room temperature.** A plate layout is provided for a record of standards and samples assayed.
5. Aspirate each well and wash, repeating the process twice for a total of three washes. Wash by filling each well with Wash Buffer (400 µL) using a squirt bottle, manifold dispenser, or autowasher. Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels.
6. Add 200 µL of Human IL-2 Conjugate to each well. Cover with a new adhesive strip. **Incubate for 2 hours at room temperature**.
7. Repeat the aspiration/wash as in step 5.
8. Add 200 µL of TMB Substrate to each well. **Incubate for 20 minutes at room temperature. Protect from light**.
9. Add 50 µL of Stop Solution to each well. Gently tap the plate to ensure thorough mixing.
10. Determine the optical density of each well within 10 minutes, using a microplate reader set to 450 nm. If wavelength correction is available, set to 540 nm or 570 nm. If wavelength correction is not available, subtract readings at 540 nm or 570 nm from the readings at 450 nm. This subtraction will correct for optical imperfections in the plate. Readings made directly at 450 nm without correction may be higher and less accurate.

11. CALCULATION OF RESULTS

Average the duplicate readings for each standard and sample and subtract the average zero standard optical density (O.D.). Create a standard curve by reducing the data using computer software capable of generating a four-parameter logistic (4-PL) curve-fit. As an alternative, construct a standard curve by plotting the mean absorbance for each standard on the y-axis against the concentration on the x-axis and draw a best fit curve through the points on the graph. The data may be linearized by plotting the log of the human IL-2 concentrations versus the log of the O.D. and the best fit line can be determined by regression analysis. This procedure will produce an adequate but less precise fit of the data.


If samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.

VIII. REFERENCES

1. Malek, T.R and I. Castro (2010) Immunity 33:153.
2. Waldman, T.A. (2006) Nat. Rev. Immunol. 6:595.
3. Malek, T.R. (2008) Annu. Rev. Immunol. 26:453.
4. Conradt, H.S. et al. (1989) J. Biol. Chem. 264:17368.
5. Taniguchi, T. et al. (1983) Nature 302:305.
6. Rosenberg, S.A. et al. (1984) Science 223:1412.
7. Smith, K.A. (1984) Annu. Rev. Immunol. 2:319.
8. Tsukaguchi, K. et al. (1995) J. Immunol. 154:1786.
9. Conlon, K. et al. (1995) Eur. J. Immunol. 25:644.
10. Hwang, I.K. et al. (2006) Brain Res. 1106:197.
11. Giestal de Araujo, E. et al. (2009) Ann. N.Y. Acad. Sci. 1153:57.
12. Kowalski, J. et al. (2004) Pol. J. Pharmacol. 56:563.
13. Eguizabal, C. et al. (2007) Int. J. Dev. Biol. 51:731.
14. Stauber, D.J. et al. (2006) Proc. Natl. Acad. Sci. USA 103:2788.

PLATE LAYOUT

Use this plate layout to record standards and samples assayed.

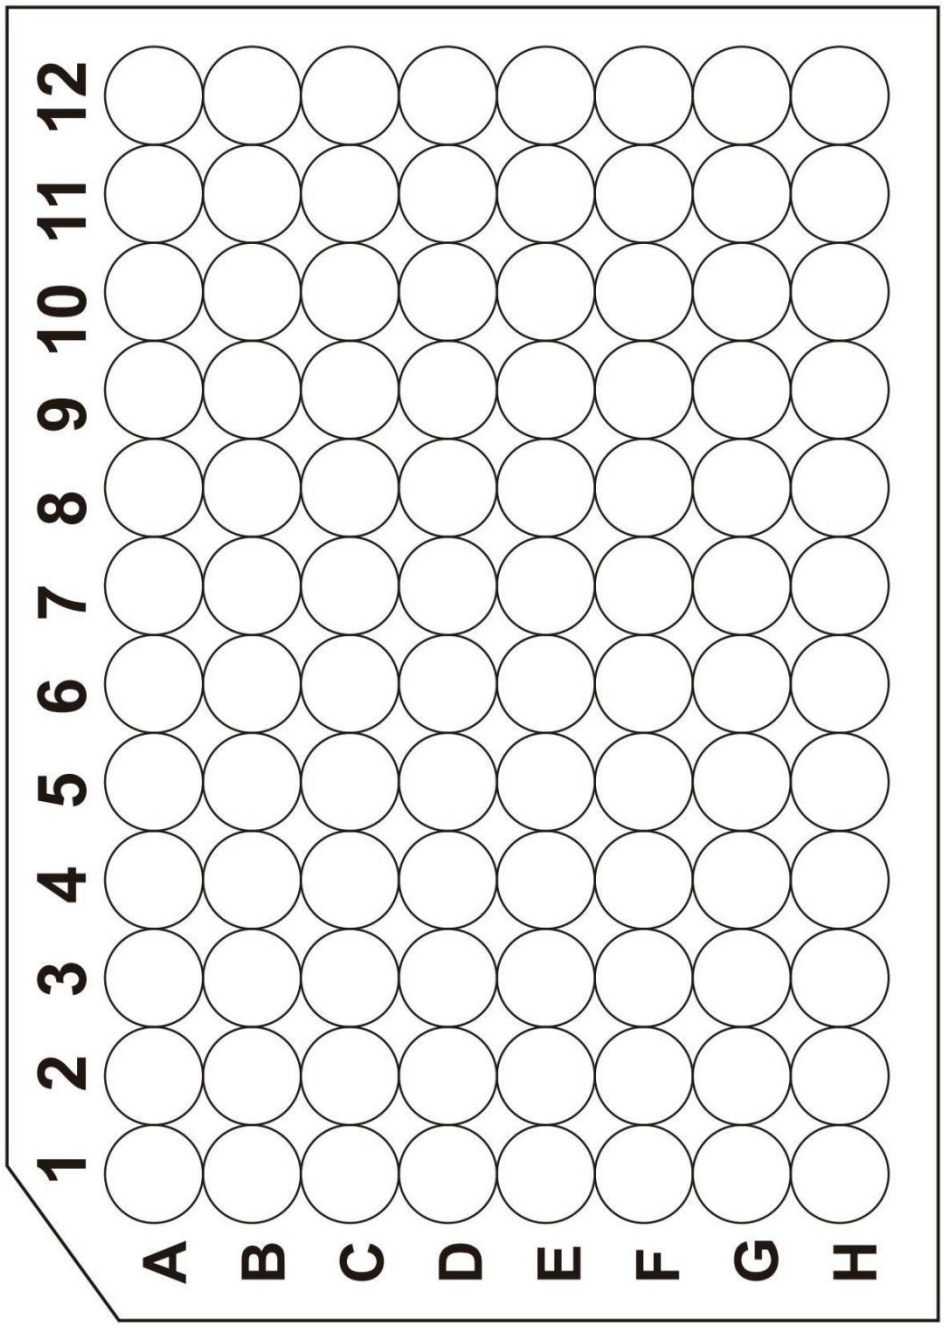

产品信息及操作手册

人 IL-2 Valukine™ ELISA 试剂盒

目录号：VAL110

适用于定量检测天然和重组人白介素 2（IL-2）的浓度

科研专用，不可用于临床诊断

Bio-Techne China Co. Ltd

P: +86 (21) 52380373 P: 8009881270 F: +86 (21) 52381001

info.cn@bio-techne.com

有效期详见试剂盒包装标签

Novus 试剂盒确保在你收货日期 3 个月内有效

版本号 202605.6

目录

I. 背景 20

II. 概述 21

III. 优势 22

IV. 实验 26

V. 试剂盒组成及储存 27

VI. 实验前准备 29

VII. 操作步骤 31

VIII. 参考文献 32

I. 背景

人白细胞介素2（IL-2），又称为T细胞生长因子（TCGF），是一个15-18 kDa大小的具有不同糖基化的α-螺旋多肽，属于常见的γ链（γc）细胞因子家族成员（1-4）。它以单体存在，半衰期很短（<30分钟）（1）。人IL-2的前体有153个氨基酸，其中包含一个20个氨基酸的信号序列，和一个133个氨基酸的成熟多肽（5, 6）。IL-2成熟蛋白包含一个在3位苏氨酸可O型糖基化的位点和三个半胱氨酸，其中的两个半胱氨酸所形成的链内二硫键是IL-2活性所必不可少的（7）。成熟的人IL-2氨基酸序列与犬、大鼠、猫和猕猴的IL-2同源性分别为73%、66%、78%和97%。虽然人IL-2与高度多态的小鼠IL-2仅有60%的氨基酸同源性，但人IL-2对小鼠细胞也具有生物活性。据报道分泌IL-2的细胞包括γδ T细胞（8）、活化的常规$CD4^+$和$CD8^+$T细胞（1, 9）、神经元（10, 11）、小胶质细胞（12）、造血干细胞（13）。

IL-2受体（IL-2R）由三个亚基构成，即一个55 kDa的CD25/IL-2Rα链、一个70 kDa的CD122/IL-2Rβ链，以及一个65 kDa的CD132/γc链（1, 3）。IL-2先与CD25结合，形成的二亚基复合物再招募CD122和CD132，形成具有四个亚基的信号复合物（1, 14）。除了能与IL-2形成复合物，CD122/IL-2Rβ也可同IL-15形成四亚基信号复合物。CD132/γc亦可成为IL-4、IL-7、IL-9、IL-15和IL-21信号的受体（1, 3）。

体外研究表明，IL-2在T细胞活化和扩增中起重要作用。在体内，IL-2是调节性T细胞（Treg）发育、维持和功能的关键，而调节性T细胞可为自身免疫性疾病提供保护。此外，IL-2也可通过调节T细胞贩运基因的表达和Th2型细胞因子的产生，从而促进其靶器官自身免疫性炎症。在$CD8^+$T细胞亚群中，IL-2是获得最佳一级反应和分化到终端效应细胞的必要关键。IL-2也促进了$CD8^+$T细胞的发育和激活成为记忆细胞（1）。

II. 概述

A. 检测原理

本实验采用双抗体夹心ELISA法。抗人IL-2抗体包被于微孔板上，样品和标准品中的人IL-2会与固定在板上的抗体结合，游离的成分被洗去；加入辣根过氧化酶标记的抗人IL-2检测抗体进行孵育。洗涤去除未结合的试剂后，加入TMB底物溶液（显色剂）。溶液颜色与结合目标蛋白成正比；加入终止液；用酶标仪测定吸光度。

B. 检测局限

- **仅供科研使用，不可用于体外诊断；**
- 该试剂盒适用于细胞培养上清样本和人血清、人血浆样本；
- 请在试剂盒有效期内使用；
- 不同试剂盒及不同批号试剂盒的组分不能混用；
- 样本值若大于标准曲线的最高值，应将样本用标准品稀释液RD5-5/RD6E稀释后重新检测；
- 检测结果的不同可由多种因素引起，包括实验人员的操作、移液器的使用方式、洗板技术、反应时间或温度、试剂盒的效期等。

III. 优势

A. 精确度

板内精确度（同一板内不同孔间的精确度）

已知浓度的三个样本，在同一板内分别检测20次，以确定板内精确度。

板间精确度（不同板之间的精确度）

已知浓度的三个样本，在不同板间分别检测20次，以确定板间精确度。

细胞培养上清

	板内精确度			板间精确度		
样本	1	2	3	1	2	3
平均值（pg/mL）	67.5	438	851	232	620	1148
标准差	2.9	14.4	26.9	23.2	34.4	45.5
CV%	4.3	3.3	3.2	10.0	5.5	4.0

血清/血浆

	板内精确度			板间精确度		
样本	1	2	3	1	2	3
平均值（pg/mL）	98.0	619	1183	250	755	1470
标准差	4.2	18.0	24.0	12.6	27.8	74.1
CV%	4.3	2.9	2.0	5.0	3.7	5.0

B. 回收率

在样本中掺入了检测范围内三个水平的人IL-2，测定其回收率。

样本类型	平均回收率（%）	范围（%）
细胞培养基（n=5）	101	96 - 107
血清（n=5）	99	89 - 114
EDTA血浆（n=5）	118	104 - 139
肝素血浆（n=5）	109	94 - 129
枸橼酸盐血浆（n=5）	105	98 - 111

C. 灵敏度

人IL-2的最低可测剂量（MDD）一般小于7 pg/mL。

MDD是根据20个重复的零标准品孔的吸光度值的平均值加两倍标准差计算得到的相对应浓度。

D. 校正

此ELISA试剂盒是针对R&D Systems®生产的大肠杆菌表达的高纯度重组人IL-2进行校准的。

NIBSC/WHO IL-2第2国际标准品(86/500)作为效价标准，在本试剂盒中进行了评估。NIBSC/WHO标准品是大肠杆菌来源的重组人IL-2。

本试剂盒评估了以下标准品：NIBSC/WHO第1批国际天然人IL-2标准品（86/504，用作效价标准）、非WHO临时参考重组人IL-2标准品（86/564）以及第2批国际标准品重组人IL-2（86/500）。所有材料均与Valukine®人IL-2标准曲线平行。若要将使用Valukine®人IL-2试剂盒测得的样品值换算为近似的NIBSC单位，请使用以下相应公式：

NIBSC（86/500）近似值（IU/mL）= 0.017 × Valukine®人IL-2测定值（pg/mL）

NIBSC（86/504）近似值（IU/mL）= 0.016 × Valukine®人IL-2测定值（pg/mL）

NIBSC（86/564）近似值（U/mL）= 0.012 × Valukine®人IL-2测定值（pg/mL）

注：*以上基于2008年9月生成的数据。*

E. 线性

不同的样本中含有或掺入高浓度的人IL-2，然后用适当的标准品稀释液RD5-5/RD6E将样本稀释到检测范围内，测定其线性。

		细胞培养基（n=5）	血清（n=5）	EDTA血浆（n=5）	肝素血浆（n=5）	枸橼酸盐血浆（n=5）
1:2	平均值/期待值（%）	102	97	100	104	100
	范围(%)	90 - 113	95 - 102	89 - 106	100 - 109	96 - 105
1:4	平均值/期待值（%）	101	94	102	104	99
	范围(%)	90 - 111	91 - 97	97 - 107	99 - 108	96 - 102
1:8	平均值/期待值（%）	99	87	99	100	97
	范围(%)	91 - 108	78 - 92	92 - 106	94 - 107	91 - 100
1:16	平均值/期待值（%）	___	___	98	95	91
	范围(%)	___	___	88 - 114	86 - 109	85 - 100

F. 样本预值

血清/血浆 - 在本检测中，对来自表面健康志愿者的 37 份血清和血浆样本进行了人 IL-2 的检测。所有样本的检测结果均低于人 IL-2 标准品的最低浓度，即 31.3 pg/mL。本研究中所用样本捐献者的病史资料不详。

G. 特异性

此ELISA法可检测天然及重组人IL-2蛋白。

将以下因子用标准品稀释液RD5-5/RD6E配制成100 ng/mL的浓度来检测与人IL-2的交叉反应。将100 ng/mL的干扰因子掺入中间范围的重组人IL-2对照品中，来检测对人IL-2的干扰。没有观察到明显的交叉反应或干扰。


Recombinant human		**Recombinant mouse**
G-CSF	IL-6	GM-CSF
GM-CSF	IL-7	IL-1β
IL-1α	IL-8	IL-2
IL-1β	LIF	IL-3
IL-2 Rα	TGF-β1	IL-4
IL-2 Rβ	TGF-β2	IL-5
IL-2 Rγ	TNF-α	IL-6
IL-3	TNF-β	IL-7
IL-4		

IV. 实验

标准曲线实例


该标准曲线数据仅供参考，每次实验应绘制其对应的标准曲线。

CELL CULTURE SUPERNATE ASSAY

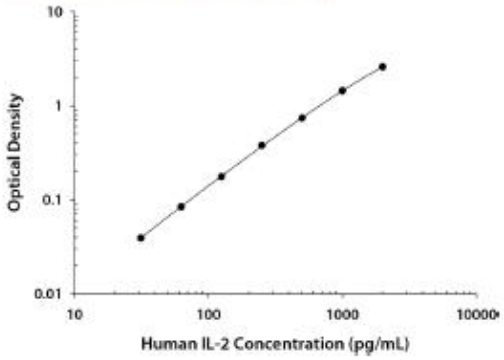

(pg/mL)	O.D.	Average	Corrected
0	0.042	0.040	——
	0.039		
31.3	0.081	0.079	0.039
	0.077		
62.5	0.127	0.124	0.084
	0.120		
125	0.221	0.216	0.176
	0.210		
250	0.404	0.418	0.378
	0.431		
500	0.802	0.779	0.739
	0.756		
1000	1.513	1.485	1.445
	1.457		
2000	2.734	2.630	2.590
	2.527		

SERUM/PLASMA ASSAY

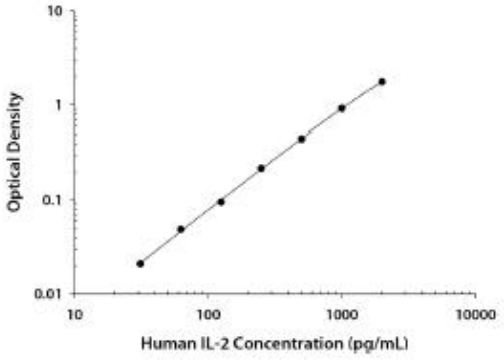

(pg/mL)	O.D.	Average	Corrected
0	0.035	0.033	——
	0.031		
31.3	0.054	0.054	0.021
	0.054		
62.5	0.084	0.082	0.049
	0.081		
125	0.121	0.129	0.096
	0.137		
250	0.247	0.252	0.219
	0.258		
500	0.474	0.482	0.449
	0.489		
1000	0.956	0.950	0.917
	0.945		
2000	1.785	1.792	1.759
	1.799		

V. 试剂盒组成及储存

A. 试剂盒组成

组成	描述	规格
Human IL-2 Microplate	包被抗人IL-2抗体的96孔聚苯乙烯板，8孔× 12条	1块板
Human IL-2 Conjugate	酶标检测抗人IL-2抗体	1瓶
Human IL-2 Standard	人IL-2标准品（冻干），参考瓶身标签进行重溶	1瓶
Assay Diluent RD1W	含防腐剂的缓冲蛋白基质。	1瓶
Calibrator Diluent RD5-5	含防腐剂的缓冲蛋白基质。*适用于细胞上清样本。*	1瓶
Calibrator Diluent RD6E	含防腐剂的动物血清。*适用于血清/血浆样本。*	1瓶
Wash Buffer Concentrate（25×）	浓缩洗涤缓冲液（25×）	1瓶
TMB Substrate	TMB ELISA底物溶液/TMB底物溶液	2瓶
Stop Solution	终止液	1瓶
Plate Sealers	封板膜	3张

B. 试剂盒储存

<table>
<tr><td>未开封试剂盒</td><td colspan="2">2-8℃储存；请在试剂盒有效期内使用</td></tr>
<tr><td rowspan="8">已打开，稀释或重溶的试剂</td><td>洗涤液（1×）</td><td rowspan="4">2-8℃储存，最多30天*</td></tr>
<tr><td>终止液</td></tr>
<tr><td>酶标检测抗体</td></tr>
<tr><td>TMB底物溶液</td></tr>
<tr><td>标准品</td><td>分装，-20℃以下冰箱储存最多30天*；
避免反复冻融。</td></tr>
<tr><td>检测液RD1W</td><td rowspan="3">2-8℃储存，最多 30 天*</td></tr>
<tr><td>标准品稀释液RD5-5</td></tr>
<tr><td>标准品稀释液RD6E</td></tr>
<tr><td>包被的微孔板条</td><td>将未用的板条放回带有干燥剂的铝箔袋内，密封；
2-8 ℃储存，最多30天*</td></tr>
</table>

*必须在试剂盒有效期内

C. 实验所需自备试验器材

- 酶标仪（可测量450nm检测波长的吸收值及540nm或570nm校正波长的吸收值）
- 高精度加液器及一次性吸头
- 蒸馏水或去离子水
- 洗瓶（喷瓶）、多通道洗板器或自动洗板机
- 500mL量筒

D. 注意事项

- 标准品稀释液RD6E含有叠氮化钠，该物质可能与铅制和铜制管道发生反应，形成具有爆炸性的金属叠氮化物。处置时请用大量水冲洗。
- 试剂盒中的一些组分含有防腐剂，可能引起皮肤过敏反应，避免吸入。
- 试剂盒中的终止液是酸性溶液，使用时请做好眼睛、手、面部及衣服的防护。

VI. 实验前准备

A. 样品收集及储存

下面列出的样本收集和储存条件仅为一般性指导原则。样本稳定性尚未经过评估。

细胞培养上清：颗粒物应离心去除；立刻检测样本。样本收集后若不及时检测，需按一次使用量分装，冻存于≤-20℃冰箱内，避免反复冻融。样本可能需要用标准品稀释液RD5-5稀释。

血清样本：用血清分离管(SST)分离血清。使血样室温凝集30分钟，然后1000×g离心15分钟。吸取血清样本之后即刻用于检测，或者分装，≤-20℃贮存备用。避免反复冻融。样本可能需要用标准品稀释液RD6E稀释。

血浆：使用 EDTA、肝素或枸橼酸盐作为抗凝剂采集血浆。采集后 30 分钟内，以 1000×g 离心 15 分钟。吸取血浆样本之后即刻用于检测，或者分装，≤-20℃贮存备用。避免反复冻融。样本可能需要用标准品稀释液 RD6E 进行稀释。


B. 检测前准备工作

使用前请将所有试剂放置于室温

洗涤液（1×）：从冰箱中取出的浓缩洗涤液可能有结晶，属于正常现象；放置室温，轻摇混匀，待结晶完全溶解后再配制洗涤液。可将20 mL浓缩洗涤液（25×）用蒸馏水或去离子水稀释配制成500 mL工作浓度的洗涤液（1×）。

人IL-2标准品：重溶体积请参考瓶身标签，使用标准品稀释液RD5-5（*用于细胞培养上清样本*）或标准品稀释液RD6E（*用于血清/血浆样本*）复溶人IL-2标准品，得到浓度为2000 pg/mL标准品母液。轻轻震摇至少15分钟，其充分溶解。

每个稀释管中加入500 µL标准品稀释液RD5-5（*用于细胞培养上清样本*）或标准品稀释液RD6E（*用于血清/血浆样本*）。将标准品母液参照下图做系列稀释，每管须充分混匀后再移液到下一管。没有稀释的标准品母液可用作标准曲线最高点（2000 pg/mL），适当的标准品稀释液RD5-5/RD6E可用作标准曲线零点（0 pg/mL）。

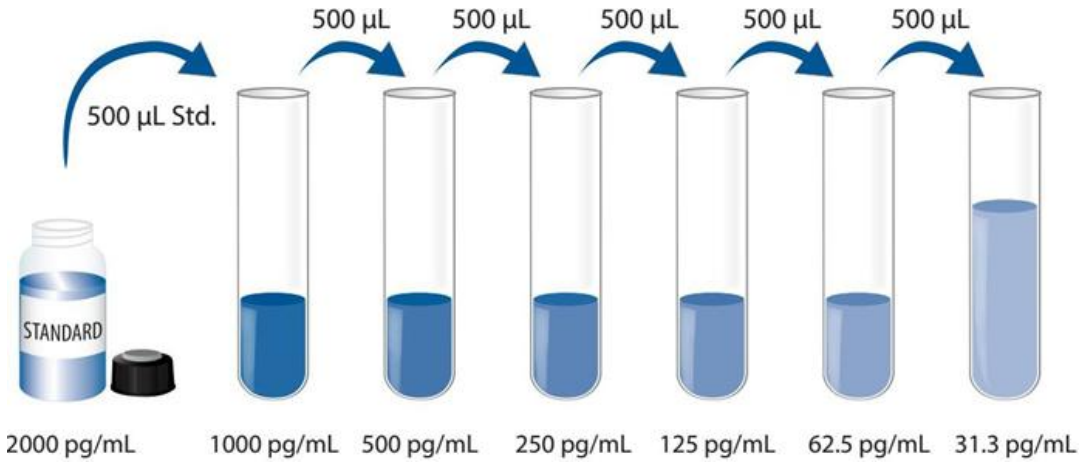

C. 技术小提示

- 当混合或重溶蛋白液时，尽量避免起沫；
- 为了避免交叉污染，配制不同浓度标准品、上样、加不同试剂都需要更换枪头。另外不同试剂请分别使用不同的移液槽；
- 建议15分钟内完成一块板的上样；
- 每次孵育时，正确使用封板膜可保证结果的准确性；
- TMB底物溶液在上板前应为无色，请避光保存；加入微孔板后，将由无色变成不同深度的蓝色；
- 终止液上板顺序应同TMB底物溶液上板顺序一致；加入终止液后，孔内颜色由蓝变黄； 若孔内有绿色，则表明孔内液体未混匀请充分混合

VII. 操作步骤

使用前请将所有试剂和样本放置于室温，建议所有的实验样本和标准品做复孔检测

1. 按照上一节的说明，准备好所有需要的试剂、样品和标准品；
2. 从已平衡至室温的密封袋中取出微孔板，未用的板条请放回铝箔袋内，重新封口；
3. 每孔加入100 µL检测液RD1W。
4. 分别将不同浓度标准品和实验样本加入相应孔中，每孔100 µL。用封板膜封住反应孔，**室温孵育2小时**。说明书提供了一张96孔模板图，可用于记录标准品和试验样本的板内位置；
5. 将板内液体吸去，使用洗瓶、多通道洗板器或自动洗板机洗板。每孔加洗涤液400 µL， 然后将板内洗涤液吸去。重复操作2次，共洗3次。每次洗板尽量吸去残留液体会有助于得到好的实验结果。最后一次洗板结束，请将板内所有液体吸干或将板倒置，在吸水纸拍干所有残留液体；
6. 在每个微孔内加入200 µL人酶标检测抗体。用封板膜封住反应孔，**室温孵育2小时**；
7. 重复第5步洗板操作；
8. 在每个微孔内加入200 µL TMB底物溶液，**室温孵育20分钟**。注意避光；
9. 在每个微孔内加入50 µL终止液，请轻拍微孔板，使溶液混合均匀；
10. 加入终止液后10分钟内，使用酶标仪测量450 nm的吸光度值，设定540 nm或570 nm作为校正波长。如果波长校正不可用，以450 nm的读数减去540 nm或570 nm的读数。这种减法将校正酶标板上的光学缺陷。没有校正而直接在450 nm处进行的读数可能会更高且更不准确；
11. 计算结果：

    将每个标准品和样品的复孔吸光值取平均值，然后减去零标准品平均OD值（O.D.），使用计算机软件作四参数逻辑（4-PL）曲线拟合创建标准曲线。另一替代方法是，通过绘制y轴上每个标准品的平均吸光值与x轴上的浓度来构建标准曲线，并通过图上的点绘制最佳拟合曲线。数据可以通过绘制人IL-2浓度的对数与O.D.的对数来线性化，并且最佳拟合线可以通过回归分析来确定。该程序将产生足够但不太精确的数据拟合。

    如果样品被稀释，从标准曲线读取的浓度必须乘以稀释倍数。

VIII. 参考文献

1. Malek, T.R and I. Castro (2010) Immunity 33:153.
2. Waldman, T.A. (2006) Nat. Rev. Immunol. 6:595.
3. Malek, T.R. (2008) Annu. Rev. Immunol. 26:453.
4. Conradt, H.S. et al. (1989) J. Biol. Chem. 264:17368.
5. Taniguchi, T. et al. (1983) Nature 302:305.
6. Rosenberg, S.A. et al. (1984) Science 223:1412.
7. Smith, K.A. (1984) Annu. Rev. Immunol. 2:319.
8. Tsukaguchi, K. et al. (1995) J. Immunol. 154:1786.
9. Conlon, K. et al. (1995) Eur. J. Immunol. 25:644.
10. Hwang, I.K. et al. (2006) Brain Res. 1106:197.
11. Giestal de Araujo, E. et al. (2009) Ann. N.Y. Acad. Sci. 1153:57.
12. Kowalski, J. et al. (2004) Pol. J. Pharmacol. 56:563.
13. Eguizabal, C. et al. (2007) Int. J. Dev. Biol. 51:731.
14. Stauber, D.J. et al. (2006) Proc. Natl. Acad. Sci. USA 103:2788.

96 孔模板图

请使用 96 孔模板图来记录标准品及样本在板内的位置

